

GeoPT18 - KPT-1, Quarz Diorite

Veranstalter: International Association of Geoanalysts and Geostandards Newsletter - GeoPT18

Ringversuchsmaterial: KPT-1, Quarz Diorite

RV geschlossen: 2006 – 4

Literatur: Proficiency Testing Report GeoPT18 (Laborcode CRB = S14)

Hauptelemente [MA%]

| | CRB | RV | 1sRV | Z-Score |
|------------------------------------|-------|-------|-------|---------|
| Na ₂ O | 2,45 | 2,61 | 0,045 | |
| MgO | 4,24 | 4,30 | 0,069 | |
| Al ₂ O ₃ | 14,41 | 14,41 | 0,193 | |
| SiO ₂ | 54,06 | 54,14 | 0,594 | |
| P ₂ O ₅ | 0,164 | 0,17 | 0,004 | |
| K ₂ O | 1,64 | 1,65 | 0,03 | |
| CaO | 7,00 | 6,89 | 0,103 | |
| TiO ₂ | 0,911 | 0,90 | 0,018 | |
| Fe ₂ O ₃ tot | 12,5 | 12,24 | 0,168 | |
| MnO | 0,155 | 0,14 | 0,004 | |

Spurenelemente [µg/g]

| | CRB | RV | 1sRV | Z-Score |
|----|-----|--------|------|---------|
| Ba | 439 | 465 | 14,7 | |
| Ce | 39 | 55 | 2,4 | |
| Cr | 158 | 152 | 5,8 | |
| Ga | 17 | 18,21 | 0,94 | |
| La | 29 | 26,9 | 1,31 | |
| Nb | 6,9 | 8,48 | 0,49 | |
| Ni | 165 | 145,7 | 5,4 | |
| Pb | 83 | 81,07 | 3,35 | |
| Rb | 70 | 64,45 | 2,65 | |
| Sr | 244 | 261,04 | 9,04 | |
| V | 181 | 197,2 | 7,12 | |
| Y | 24 | 25,82 | 1,27 | |
| Zn | 115 | 120,24 | 4,68 | |
| Zr | 138 | 158,12 | 5,9 | |

Legende

CRB: Ergebnisse CRB – **RV:** Ergebnisse Ringversuch -- **1s-RV:** Standardabweichung Ringversuch

Z-Score: Differenz des Messwertes vom Mittelwert des Ringversuchs -- * Wert nicht zertifiziert

GEOPT18 - AN INTERNATIONAL PROFICIENCY TEST FOR ANALYTICAL GEOCHEMISTRY LABORATORIES - REPORT ON ROUND 18 / Jan 2006 (Quartz diorite, KPT-1)

**Peter C. Webb^{1*}, Michael Thompson², Philip J. Potts¹
and L. Paul Bedard³**

¹Department of Earth Sciences, The Open University, Walton Hall, Milton Keynes, MK7 6AA, UK.

²Department of Chemistry, Birkbeck College, Gordon House, London, WC1H 0PP, UK.

³Sciences Appliquées, Université du Québec à Chicoutimi, Chicoutimi, Quebec, G7H 2B1, Canada.

*Corresponding author: e-mail p.c.webb@open.ac.uk

Keywords: Proficiency testing, quality assurance, GeoPT, GeoPT18 round, KPT-1, quartz diorite

Abstract

Results are presented for GeoPT18, round eighteen of the GeoPT international proficiency testing programme for analytical geochemistry laboratories. The sample distributed for this round was KPT-1, a quartz diorite, supplied by Dr Paul Bedard, Quebec. In this report, contributed data are listed, together with an assessment of assigned values, z-scores and charts showing both the distribution of contributed results and the overall performance of participating laboratories.

Introduction

This eighteenth round of the international proficiency testing programme, GeoPT18, was conducted in a similar manner to earlier rounds. The programme is designed to be part of the routine quality assurance scheme of analytical geochemistry laboratories and the aims of the programme can be reviewed at <http://www.geoanalyst.org/geopt.html>. The programme is organised by the International Association of Geoanalysts and is conducted in accordance with a published protocol (<http://www.geoanalyst.org/GeoPt-protocol.pdf>). The overall aim of the programme is to provide participating laboratories with z-score information for

each reported elemental determination, from which the laboratories can decide whether the quality of their data is satisfactory in relation to both their chosen fitness-for-purpose criterion and results submitted by all the other laboratories contributing to the round and, therefore, choose to take corrective action if this appears justified.

Full details of the programme have been included in reports of previous rounds, the current publication status of which is listed in Appendix 1.

Steering Committee for Round 18: M. Thompson (Chair), P.J. Potts (Secretary) and P.C. Webb.

Sample: KPT-1, a quartz diorite, was supplied ready packaged by Dr L. Paul Bedard (Quebec).

The sample was tested for homogeneity in accordance with published protocol and based on WDXRF determinations of 10 packets selected at random, each of which was analysed in duplicate. A test for lack of sufficient homogeneity has been carried out in respect of the elements (SiO₂, TiO₂, Al₂O₃, Fe₂O, MnO, MgO, CaO, Na₂O, K₂O, LOI, Rb, Sr, Y, Zr, Nb, Ba, Pb, Th, U, Sc, V, Cr, Co, Ni, Cu, Zn, Ga, Mo, As, S),

according to the modified procedure mentioned in the GeoPT Protocol. Lack of sufficient homogeneity was detected in one analyte, namely cobalt. It was therefore considered that this material was suitable for use in the GeoPT proficiency testing programme.

Timetable for GeoPT18:

Distribution of sample: October 2006.

Deadline for submission of analytical results: 15th December 2005.

Distribution of draft report: February 2006

Submission of results

Results submitted by the seventy-six laboratories that participated in this round are listed in Table 1. All of these data were used for the assessment of assigned values.

Assigned values

Following procedures described in earlier rounds, a robust statistical procedure was used to derive assigned concentration values [X_a], these being judged to be the best estimates of the true composition of this sample. Data in Table 2 lists assigned values for 10 major components and 39 trace elements. Values were assigned on the basis that: (i) sufficient laboratories had contributed data for an element, (ii) the statistical assessment gave confidence that the results showed a central portion approximating to a normal distribution. Part of this assessment involved examining a bar chart for each element to judge the distribution of results. Bar charts for elements/species shown in Figure 1 were judged to have satisfactory distributions, namely:

SiO₂, TiO₂, Al₂O₃, Fe₂O₃T, MnO, MgO, CaO, Na₂O, K₂O, P₂O₅, Ba, Be, Bi, Ce, Cr, Cs, Dy, Er, Eu, Ga, Gd, Hf, Ho, La, Li, Lu, Mo, Nb, Nd, Pb, Pr, Rb, Sb, Sc, Se, Sm, Sn, Sr, Ta, Tb, Th, Tl, Tm, U, V, Y, Yb, Zn, and Zr.

Charts in Figure 2 show distribution data for elements for which z-scores are plotted for guidance only, the statistical analysis was sufficiently unsatisfactory to

be able to assign values. Consequently, values were not assigned to the following elements/species: CO₂, Fe(II)O, LOI, Ag, As, Au, Cd, Co, Cu, Ge, Pd and W.

For the following elements either insufficient data were reported (H₂O⁺, Cl, F, Pt, S and Te) or the distribution was sufficiently unsatisfactory (S) to allow any assessment to be made.

Z-score analysis

As in previous rounds, laboratories were invited to choose one of two performance standards against which their analytical results would be judged:

Data quality 1 for laboratories working to a 'pure geochemistry' standard of performance, where analytical results are designed for geochemical research and where care is taken to provide data of high precision and accuracy, sometimes at the expense of a reduced sample throughput rate.

Data quality 2 for laboratories working to an 'applied geochemistry' standard of performance, where, although precision and accuracy are still important, the main objective is to provide results on large numbers of samples collected, for example, as part of geochemical mapping projects or geochemical exploration programmes.

The target standard deviation (H_a) for each element assessed was calculated from a modified form of the Horwitz function as follows:

$$H_a = k.X_a^{0.8495}$$

Where X_a is the concentration of the element expressed as a *fraction*, and the factor $k = 0.01$ for pure geochemistry labs and $k=0.02$ for applied geochemistry labs.

Z-scores were calculated for each elemental result submitted by each laboratory from:

$$z = [X - X_a] / H_a$$

where

X is the contributed result, X_a is the assigned value and H_a is the target standard deviation.

Z-score results are listed in Table 3 and participating laboratories are invited to assess their performance using the following criterion:–

Z-score results in the range $-2 < z < 2$ are considered to be 'satisfactory' (in the sense that no action is called for by the participant). If the z-score for any element falls outside this range, contributing laboratories are advised to examine their procedures to ensure that determinations are not subject to unsuspected analytical bias.

Overall performance

A summary of the overall performance of individual laboratories in this round is plotted in Figure 3 as a multiple z-score chart. In this chart, the z-score performance for each element is distinguished by symbols that make it simple to identify whether the results were satisfactory or gave z-scores that exceeded the action limits. This chart is designed to help individual laboratories to judge their overall performance in this proficiency testing round.

For this sample there were a larger range of elements than usual for which no assigned value could be given. There also appear to be many higher z-scores than is usual. Initial indications are that the high Ca content of this sample may pose problems that are not usually encountered, and possibly that more elements than usual were close to detection limits for some techniques.

Participation in future rounds

The benefit from proficiency testing arises from regular participation and laboratories are invited to contribute to the GeoPT19 round, the sample for which will be distributed during March 2006.

Acknowledgments

The authors thank John Watson and Liz Lomas (OU) for valued assistance with the production of this report. The GeoPT programme is organised on behalf of the International Association of Geoanalysts.

Appendix 1

Publication status of proficiency testing reports

GeoPT1

Thompson M., Potts P.J., Kane J.S. and Webb P.C. (1996)
GeoPT1. International proficiency test for analytical geochemistry laboratories - Report on round 1. Geostandards Newsletter: The Journal of Geostandards and Geoanalysis, 20, 295-325.

GeoPT2

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson, J.S. (1998)
GeoPT2. International proficiency test for analytical geochemistry laboratories - Report on round 2. Geostandards Newsletter: The Journal of Geostandards and Geoanalysis, 22 127-156.

GeoPT3

Thompson M., Potts P.J., Kane J.S. and Chappell B.W. (1999a)
GeoPT3. International proficiency test for analytical geochemistry laboratories - Report on round 3. Geostandards Newsletter: The Journal of Geostandards and Geoanalysis, 23, 87-121.

GeoPT4

Thompson M., Potts P.J., Kane J.S., Webb P.C. and Watson J.S. (1999b)
GeoPT4. International proficiency test for analytical geochemistry laboratories - Report on round 4. Published in the electronic version of Geostandards Newsletter: The Journal of Geostandards and Geoanalysis (Summer 2000).

GeoPT5

Thompson M., Potts P.J., Kane J.S., and Wilson S. (1999c)
GeoPT5. International proficiency test for analytical geochemistry laboratories - Report on round 5. Published in the electronic version of Geostandards Newsletter: The Journal of Geostandards and Geoanalysis (Summer 2000).

GeoPT6

Potts P.J., Thompson M., Kane J.S., Webb P.C. and Carignan J. (2000)
GEOPT6 - an international proficiency test for analytical geochemistry laboratories - report on round 6 (OU-3: Nanhonon microgranite) and 6A (CAL-S: CRPG limestone). International Association of Geoanalysts: Unpublished report.

GeoPT7

Potts P.J., Thompson M., Kane J.S., and Petrov L.L. (2000)
GEOPT7 - an international proficiency test for analytical geochemistry laboratories - report on round 7 (GBPG-1 Garnet-biotite plagiogneiss). International Association of Geoanalysts: Unpublished report.

GeoPT8

Potts P.J., Thompson M., Kane J.S., Webb, P.C. and Watson J.S. (2000)
GEOPT8 - an international proficiency test for analytical geochemistry laboratories - report on round 8 / February 2001 (OU-4 Penmaenmawr microdiorite). International Association of Geoanalysts: Unpublished report.

GeoPT9

Potts P.J., Thompson M., Webb, P.C. and Watson J.S. (2001)
GEOPT9 - an international proficiency test for analytical geochemistry laboratories - report on round 9 / July 2001 (OU-6

Penrhyn slate). International Association of Geoanalysts: Unpublished report.

GeoPT10

Potts P.J., Thompson M., Webb, P.C., Watson J.S. and Wang Yimin (2001)
GEOPT10 - an international proficiency test for analytical geochemistry laboratories - report on round 10 / December 2001 (CH-1 Marine sediment). International Association of Geoanalysts: Unpublished report.

GeoPT11

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Watson J.S. (2002)
GEOPT11 - an international proficiency test for analytical geochemistry laboratories - report on round 11 / July 2002 (OU-5 Leaton dolerite). International Association of Geoanalysts: Unpublished report.

GeoPT12

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Batjargal B. (2003)
GEOPT12 - an international proficiency test for analytical geochemistry laboratories - report on round 12 / January 2003 (GAS Serpentinite). International Association of Geoanalysts: Unpublished report.

GeoPT13

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and Kaspar H.U. (2003)
GEOPT13 - an international proficiency test for analytical geochemistry laboratories - report on round 13 / July 2003 (Köln Loess). International Association of Geoanalysts: Unpublished report.

GeoPT14

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and B. Batjarga (2004)
GeoPT14 - an international proficiency test for analytical geochemistry laboratories - report on round 14 / January 2004 (OShBO - alkaline granite). International Association of Geoanalysts: Unpublished report.

GeoPT15

Potts P.J., Thompson M., Chenery S.R., Webb, P.C. and WANG Yimin (2004)
GeoPT15 - an international proficiency test for analytical geochemistry laboratories - report on round 15 / June 2004 (Ocean floor sediment MSAN). International Association of Geoanalysts: Unpublished report.

GeoPT16

Potts P.J., Thompson M., Webb, P.C. and S.Wilson (2005)
GeoPT16 - an international proficiency test for analytical geochemistry laboratories - report on round 16 / February 2005 (Nevada basalt, BNV-1). International Association of Geoanalysts: Unpublished report.

GeoPT17

Potts P.J., Thompson M., Webb, P.C. and J. Nicholas Walsh (2005)
GeoPT17 - an international proficiency test for analytical geochemistry laboratories - report on round 17 / July 2005 (Calcareous sandstone, OU-8). International Association of Geoanalysts: Unpublished report.

| Table 1 | | GeoPT18 Analytical results submitted (Dec. 2005) | | | | | | | | | | | | |
|------------------|---------|--|-------|--------|--------|-------|-------|--------|-------|--------|-------|-------|-------|-------|
| | | Quartz diorite KPT-1 | | | | | | | | | | | | |
| Round identifier | | S13 | S14 | S15 | S16 | S17 | S18 | S19 | S19 | S20 | S21 | S22 | S22 | S23 |
| Sample | | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Data quality | | 2 | 2 | 1 | 1 | 2 | 1 | 1 | 2 | 2 | 2 | 1 | 2 | 1 |
| SiO2 | % m/m | | 54.06 | 54.407 | | 47.8 | | 55.22 | | 55.31 | 54.39 | 54.18 | | |
| TiO2 | % m/m | 0.86 | 0.911 | 0.921 | 1.096 | 0.84 | | 1 | | 0.9 | 0.89 | 0.89 | | |
| Al2O3 | % m/m | 13.97 | 14.41 | 14.505 | 18.29 | 21.7 | | 14.38 | | 14.61 | 14.68 | 14.44 | | |
| Fe2O3 | % m/m | 11.59 | 12.5 | 12.215 | 13.81 | 11.9 | | 12.260 | | 12.15 | 12.29 | 12.35 | | |
| Fe(II)O | % m/m | | | 7.99 | | | | | | | | | | |
| MnO | % m/m | 0.145 | 0.155 | 0.136 | 0.1666 | 0.155 | | 0.141 | | 0.1372 | 0.14 | 0.13 | | |
| MgO | % m/m | 4.34 | 4.24 | 4.336 | 4.692 | | | 4.291 | | 4.35 | 4.47 | 4.60 | | |
| CaO | % m/m | 6.9 | 7 | 6.826 | 7.636 | 7.35 | | 7.049 | | 6.87 | 6.93 | 6.89 | | |
| Na2O | % m/m | 2.58 | 2.45 | 2.65 | 2.829 | | | 2.426 | | 2.51 | 2.55 | 2.74 | | |
| K2O | % m/m | 1.74 | 1.64 | 1.637 | 4.024 | 1.93 | | 1.672 | | 1.66 | 1.66 | 1.52 | | |
| P2O5 | % m/m | 0.165 | 0.164 | 0.176 | 0.2456 | | | 0.138 | | 0.171 | 0.15 | 0.13 | | |
| H2O+ | % m/m | | | | | | | | | | | | | |
| CO2 | % m/m | | | | | | | | | | | | | |
| LOI | % m/m | | 1.43 | 1.2 | | | | 1.52 | | 1.49 | | 1.50 | | |
| Ag | mg kg-1 | 0.671 | | | | | | 0.4 | | | 0.73 | | | |
| As | mg kg-1 | 1.745 | | | 4.614 | | | | 1.6 | | 2.6 | | | |
| Au | mg kg-1 | | | | 6.033 | | | | | | | | | |
| B | mg kg-1 | | | | | | | | | | | | | |
| Ba | mg kg-1 | 465.144 | 439 | 456.3 | 608 | 474 | 458 | | 453 | 440 | 479 | 470 | | 456 |
| Be | mg kg-1 | | | | | | | 1.1 | | | 1.37 | | | |
| Bi | mg kg-1 | 0.640 | | | | | | | 1.7 | | | | | 0.81 |
| Br | mg kg-1 | | | | | | | | | | | | | |
| Cd | mg kg-1 | 0.359 | | | 8.57 | | | 0.7 | | | 0.44 | | | |
| Ce | mg kg-1 | 53.647 | 39 | 52.78 | | 54 | 53.7 | | 60.3 | | 56.5 | 66 | | 53 |
| Cl | mg kg-1 | 75.204 | | | | 16000 | | | | | | | | |
| Co | mg kg-1 | | 62 | 77.02 | 66.92 | | 80.6 | | 86.4 | | 85.7 | | 51 | 72 |
| Cr | mg kg-1 | 139.187 | 123 | 148.97 | 480 | 233 | 152 | | 167 | | 170 | 163 | | 139 |
| Cs | mg kg-1 | 4.312 | 3.5 | 4.256 | 21.94 | | 4.03 | | | | 5.19 | | | 4.2 |
| Cu | mg kg-1 | 1204.353 | 1040 | 1165 | 2051 | 1050 | 906 | | 1105 | | 1310 | | 780 | |
| Dy | mg kg-1 | 4.371 | | 4.46 | | | 4.47 | 3.06 | | | | | | 4.4 |
| Er | mg kg-1 | 2.626 | | 2.691 | | | 2.75 | 1.64 | | | | | | 2.7 |
| Eu | mg kg-1 | 1.213 | | 1.203 | | | 1.17 | 1.07 | | | | | | 1.2 |
| F | mg kg-1 | | | | | | | | | | | | | |
| Ga | mg kg-1 | 17.874 | 17 | 18.55 | | 17 | 19 | | 18 | | 21.7 | 16 | | 19 |
| Gd | mg kg-1 | 4.386 | | 4.622 | | | 4.89 | 3.72 | | | | | | 4.6 |
| Ge | mg kg-1 | | | | | | | | | | 4 | | | 1.4 |
| Hf | mg kg-1 | | | 4.342 | | | 4.02 | | 3.1 | | | 4.7 | | 3.7 |
| Hg | mg kg-1 | | | | | | | | | | | | | |
| Ho | mg kg-1 | | | 0.958 | | | 0.947 | 0.57 | | | | | | 0.91 |
| I | mg kg-1 | | | | | | | | | | | | | |
| In | mg kg-1 | | | | | | | | | | | | | |
| Ir | mg kg-1 | | | | | | | | | | | | | |
| La | mg kg-1 | 26.039 | 29 | 26.19 | 40.95 | 24 | 24.8 | | 29 | | 28.7 | | | 26 |
| Li | mg kg-1 | | | | 102 | | | 28.6 | | | | | | |
| Lu | mg kg-1 | 0.380 | | 0.437 | 0.8222 | | 0.4 | 0.2 | | | | | | 0.41 |
| Mo | mg kg-1 | 0.288 | 1.6 | | 3.852 | | | | 1.8 | | 2.17 | | | 0.3 |
| N | mg kg-1 | | | | | | | | | | | | | |
| Nb | mg kg-1 | | 6.9 | 9.41 | | 5 | 7.87 | | 7.9 | | | 9 | | 7.7 |
| Nd | mg kg-1 | 24.148 | 22 | 24.36 | | 23 | 24.1 | | 23.1 | | | 22 | | 24 |
| Ni | mg kg-1 | 1079.563 | 760 | 1214.7 | 1293 | 850 | 1016 | | 901 | | 1185 | 1210 | | |
| Os | mg kg-1 | | | | | | | | | | | | | |
| Pb | mg kg-1 | 81.830 | 52 | 79.35 | 92.34 | 90 | | | 82.2 | | | | 59 | 77 |
| Pd | mg kg-1 | | | | | | | | | | | | | |
| Pr | mg kg-1 | 6.181 | | 6.39 | | | 6.11 | 7.01 | | | | 6.4 | | 6.2 |
| Pt | mg kg-1 | | | | | | | | | | | | | |
| Rb | mg kg-1 | 53.235 | 70 | 65.07 | | 60 | 59.9 | | 60.2 | | 64.4 | 63 | | 58 |
| Re | mg kg-1 | 13.710 | | | | | | | | | | | | |
| Rh | mg kg-1 | | | | | | | | | | | | | |
| Ru | mg kg-1 | | | | | | | | | | | | | |
| S | mg kg-1 | | | | 10370 | 8300 | | | | 9990 | | | 3680 | |
| Sb | mg kg-1 | 9.965 | 2.8 | | 14.23 | | | 4.3 | | | 11.65 | | | 10 |
| Sc | mg kg-1 | 23.258 | 27 | 25.16 | 24.93 | | | | 31 | | | 23 | | 25 |
| Se | mg kg-1 | 2.700 | | | 2.5 | | | 5.3 | | | | | | |
| Sm | mg kg-1 | 4.808 | 3 | 4.929 | | | 4.76 | 4.52 | | | | | | 4.3 |
| Sn | mg kg-1 | 18.832 | 18 | | 29.08 | | | | 18.2 | | 19.8 | | | 19 |
| Sr | mg kg-1 | 169.053 | 244 | 263.19 | 265.8 | 260 | 259 | | 258 | 310 | 271 | 240 | | 226 |
| Ta | mg kg-1 | | | 0.555 | | | 0.606 | | | | | | | 0.61 |
| Tb | mg kg-1 | 0.691 | | 0.762 | | | 0.725 | 0.53 | | | | | | 0.71 |
| Te | mg kg-1 | | | | | | | | | | | | | |
| Th | mg kg-1 | 6.937 | 8 | 6.45 | 13.69 | | 6.71 | | 8.4 | | 7.6 | | | 6.8 |
| Tl | mg kg-1 | 0.485 | | | | | | | | | 0.51 | | | 0.51 |
| Tm | mg kg-1 | | | 0.418 | | | 0.395 | 0.24 | | | | | | 0.39 |
| U | mg kg-1 | 1.690 | 4 | 1.707 | 4.071 | | 1.68 | | 4.4 | | 1.8 | | | 1.6 |
| V | mg kg-1 | 191.026 | 181 | 191.86 | 240 | 210 | 200 | | 200 | | 217 | 203 | | 189 |
| W | mg kg-1 | | | | 1.583 | | | | 4.5 | | | | | 1.1 |
| Y | mg kg-1 | | 24 | 27.98 | 44.29 | 23 | 23.7 | | 26.6 | | 26.8 | 26 | | 24 |
| Yb | mg kg-1 | 2.552 | | 2.715 | | | 2.73 | 0.84 | | | | | | 2.7 |
| Zn | mg kg-1 | 117.870 | 115 | 116.57 | 164.2 | 1120 | | | 113 | | 120 | 125 | | 148 |
| Zr | mg kg-1 | 119.027 | 138 | 175.26 | 345.6 | 145 | 153 | | 158 | | 152 | 175 | | 130 |

| Table 1 | | GeoPT18 Analytical results submitted (Dec. 2005) | | | | | | | | | | | | |
|------------------|---------|---|-------|--------|-------|-------|--------|-------|-------|-------|-------|--------|--------|---------|
| | | Quartz diorite KPT-1 | | | | | | | | | | | | |
| Round identifier | | S23 | S24 | S25 | S25 | S26 | S27 | S28 | S28 | S29 | S30 | S31 | S32 | S33 |
| Sample | | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Data quality | | 2 | 2 | 1 | 2 | 1 | 2 | 1 | 2 | 2 | 1 | 1 | 2 | 1 |
| SiO2 | % m/m | | 54.6 | 55.24 | | 54.46 | 53.01 | 54.16 | | 53.3 | 54.50 | 51.04 | 53.678 | 54.0772 |
| TiO2 | % m/m | 0.84 | 0.83 | 0.896 | | 0.89 | 0.924 | 0.93 | | 0.8 | 0.86 | 0.8722 | 0.906 | 0.8742 |
| Al2O3 | % m/m | | 13.9 | 14.484 | | 14.34 | 14.05 | 14.74 | | 14.51 | 14.48 | 12.18 | 14.451 | 14.4857 |
| Fe2O3 | % m/m | | 12.7 | 12.346 | | 12.05 | 11.59 | 12.53 | | 12 | 12.14 | 12.06 | 12.329 | 12.2663 |
| Fe(II)O | % m/m | | | 8.85 | | 8.16 | | | | | | | 7.99 | 7.9187 |
| MnO | % m/m | 0.13 | 0.15 | 0.146 | | 0.152 | 0.139 | | 0.144 | 0.13 | 0.144 | 0.1379 | 0.136 | 0.1473 |
| MgO | % m/m | | 4.43 | 4.399 | | 4.52 | 4.23 | | 4.21 | 5.4 | 4.24 | 4.292 | 4.393 | 4.3428 |
| CaO | % m/m | | 6.97 | 6.888 | | 7.15 | 6.59 | 6.92 | | 6.85 | 6.81 | 6.687 | 6.876 | 6.8253 |
| Na2O | % m/m | | 2.56 | 2.63 | | 2.54 | 2.49 | | | 2.77 | 2.61 | 1.838 | 2.582 | 2.6572 |
| K2O | % m/m | | 1.61 | 1.632 | | 1.66 | 1.57 | | | 1.7 | 1.62 | 1.578 | 1.65 | 1.6563 |
| P2O5 | % m/m | | 0.18 | 0.167 | | 0.147 | 0.164 | | 0.163 | 0.194 | 0.156 | 0.1602 | 0.171 | 0.1643 |
| H2O+ | % m/m | | | | | 1.51 | | | | 0.27 | | | | |
| CO2 | % m/m | | | | | 0.67 | | | | | | | | |
| LOI | % m/m | | 1.52 | 1.28 | | 1.55 | 1.91 | | 1.64 | 1.88 | 2.05 | | 1.5 | |
| Ag | mg kg-1 | | | | | | | | 1.100 | | | | | 0.564 |
| As | mg kg-1 | | | | | 1.61 | 1.51 | | 4.4 | | | 4.2 | | 3.783 |
| Au | mg kg-1 | | | | | | | | 0.013 | | | | | |
| B | mg kg-1 | | | | | | | | 33 | | | | | |
| Ba | mg kg-1 | | 422 | 471 | | 417 | 518.5 | | 457.0 | 430 | | 474.3 | 455 | 460 |
| Be | mg kg-1 | | | | | 2.15 | | | 1.67 | | | | | 1.33 |
| Bi | mg kg-1 | | | | | 0.97 | 2.6 | | | | | 1.6 | | |
| Br | mg kg-1 | | | | | | | | | | | | | |
| Cd | mg kg-1 | 0.45 | | | | | 0.21 | | 0.50 | 0.37 | | 2 | | |
| Ce | mg kg-1 | | 53 | | 52 | 58.9 | | 62.5 | | | | 55.7 | 73 | 52.215 |
| Cl | mg kg-1 | | | | | | 392.1 | | | | | | | |
| Co | mg kg-1 | | 58.6 | | | 79 | 68.1 | | 80 | 80.8 | | | 61 | |
| Cr | mg kg-1 | | 171 | 171.5 | | 169 | 131.6 | | 145 | 164 | | 130.4 | 170 | 161.8 |
| Cs | mg kg-1 | | 3.73 | | | | 7.2 | | 3 | | | 5 | 5.31 | 5.068 |
| Cu | mg kg-1 | 1030 | 1460 | 915 | | 1263 | 866.4 | 1106 | | 1251 | | 1242 | 955 | 890 |
| Dy | mg kg-1 | | 4.34 | | | 5.04 | | 4.57 | | | | | 5.78 | 4.65 |
| Er | mg kg-1 | | 2.52 | | | 2.78 | | 2.84 | | | | | 4 | 2.885 |
| Eu | mg kg-1 | | 1.28 | | | 1.22 | | 1.32 | | | | | 1.38 | 1.22 |
| F | mg kg-1 | | | | | 720 | | | 400 | 460 | | | | 556.6 |
| Ga | mg kg-1 | | | | | | 18.9 | 17.7 | | 16.4 | | 16.4 | | 19.116 |
| Gd | mg kg-1 | | 4.33 | | | 5.80 | | | 4.63 | | | | 6.44 | 4.646 |
| Ge | mg kg-1 | | | | | | | 1.41 | | | | | | 1.4 |
| Hf | mg kg-1 | | 4.33 | | | | 4.41 | | 4.52 | | | | 3.93 | 4.916 |
| Hg | mg kg-1 | | | | | 0.00 | | | 0.007 | | | | | |
| Ho | mg kg-1 | | 1.0 | | | 1.38 | | 0.94 | | | | | 1.23 | 0.986 |
| I | mg kg-1 | | | | | | | | | | | | | |
| In | mg kg-1 | | | | | | | | | | | | | |
| Ir | mg kg-1 | | | | | | | | | | | | | |
| La | mg kg-1 | | 26.5 | | 25 | 28.3 | 35.1 | 29.4 | | | | 23.6 | 32 | 25.256 |
| Li | mg kg-1 | | | | | 32.5 | | 34 | | | | | | |
| Lu | mg kg-1 | | 0.42 | | | 0.56 | | 0.42 | | | | | 0.67 | 0.47 |
| Mo | mg kg-1 | | 1.1 | | | | 1.82 | | 1.50 | | | | 1.15 | 1.8 |
| N | mg kg-1 | | | | | | | | | | | | | |
| Nb | mg kg-1 | | 7.30 | 8.3 | | 9.0 | 9.38 | | 7 | 9.4 | | 8.4 | 9 | 8 |
| Nd | mg kg-1 | | 24.0 | | | 26.4 | | 25.8 | | | | | 31.3 | 25.068 |
| Ni | mg kg-1 | 1050 | 1381 | 895.1 | | 1203 | 1021 | 1226 | | 724 | | 1130 | 772 | 861.6 |
| Os | mg kg-1 | | | | | | | | | | | | | |
| Pb | mg kg-1 | | 126 | 83.1 | | 83 | 7661 | | 64 | 67.5 | | 78.5 | 76 | 83.73 |
| Pd | mg kg-1 | | | | | | | | 0.062 | | | | | |
| Pr | mg kg-1 | | 6.26 | | | 6.7 | | 6.8 | | | | | 8.06 | 6.173 |
| Pt | mg kg-1 | | | | | | | | | | | | | |
| Rb | mg kg-1 | | 56.7 | 61.2 | | 58 | 63.15 | 55 | | 54.5 | | 55.6 | 83 | 60.3 |
| Re | mg kg-1 | | | | | | | | | | | | | |
| Rh | mg kg-1 | | | | | | | | | | | | | |
| Ru | mg kg-1 | | | | | | | | | | | | | |
| S | mg kg-1 | | | | | 10890 | 8273.1 | | | | | 8337 | | 9536.85 |
| Sb | mg kg-1 | | 10.0 | | | 7.38 | 6.1 | 12.5 | | | | 13.5 | | 9.983 |
| Sc | mg kg-1 | | 23.8 | | | | 21.1 | 27.9 | | | | | | 25 |
| Se | mg kg-1 | | | | | | | | | | | 0.6 | | |
| Sm | mg kg-1 | | 5.0 | | | 4.68 | | 4.86 | | | | 6.7 | 6.5 | 5.026 |
| Sn | mg kg-1 | | 17.5 | | | 9 | 17 | | 17.30 | | | 21.5 | 27.51 | 20.116 |
| Sr | mg kg-1 | | 239 | 262.2 | | 254 | 273.2 | | 278 | 241 | | 235.9 | 306 | 264.24 |
| Ta | mg kg-1 | | 0.64 | | | | 0.61 | | | | | | 1.72 | 0.483 |
| Tb | mg kg-1 | | 0.76 | | | | | 0.81 | | | | | 1.11 | 0.688 |
| Te | mg kg-1 | | | | | | | | | | | | | |
| Th | mg kg-1 | | 7.2 | | 10 | | 8.69 | 7.46 | | 8.2 | | 7.8 | 5 | 6.283 |
| Tl | mg kg-1 | | | | | | | | 0.60 | | | 1.5 | | |
| Tm | mg kg-1 | | 0.46 | | | 0.40 | | 0.43 | | | | | 0.44 | |
| U | mg kg-1 | | 1.89 | | 1 | | 1.19 | 1.98 | | | | 3.1 | 2.35 | 1.766 |
| V | mg kg-1 | | 201 | 205.8 | | 187 | 208.9 | | 201 | 202 | | 191.9 | 187 | 209.4 |
| W | mg kg-1 | | 1.46 | | | | | | 1.06 | | | | | |
| Y | mg kg-1 | | 27.5 | 27.7 | | 28.0 | 28.08 | 28.6 | | 23.4 | | 25 | 50 | 21.35 |
| Yb | mg kg-1 | | 2.63 | | | 3.64 | | 2.79 | | | | 19.4 | 3.8 | 2.808 |
| Zn | mg kg-1 | | 138 | 119.9 | | 134 | 161.8 | | 134 | 108 | | 115.4 | 199 | 122.6 |
| Zr | mg kg-1 | | 166 | 156.1 | | 151 | 165.1 | 195 | | 147 | | 153.3 | 122 | 156.8 |

| Table 1 | | GeoPT18 Analytical results submitted (Dec. 2005) | | | | | | | | | | | | |
|------------------|---------|--|---------|-------|-------|-------|-------|-------|-------|---------|--------|-------|-------|-------|
| | | Quartz diorite KPT-1 | | | | | | | | | | | | |
| Round identifier | | S34 | S35 | S36 | S37 | S38 | S39 | S39 | S40 | S41 | S42 | S43 | S44 | S44 |
| Sample | | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Data quality | | 1 | 1 | 2 | 2 | 2 | 1 | 2 | 1 | 2 | 1 | 2 | 1 | 2 |
| SiO2 | % m/m | 54.48 | 54.8 | 52.04 | 54.33 | 53.24 | | 54.58 | 53.44 | 54.8 | | 54.47 | | |
| TiO2 | % m/m | 0.89 | 0.951 | 0.9 | 0.9 | 0.852 | | 0.91 | 0.86 | 0.925 | 0.94 | 0.93 | 0.87 | |
| Al2O3 | % m/m | 14.61 | 13.4 | 16.26 | 14.57 | 14.13 | | 14.46 | 14.08 | 14.45 | | 14.31 | 14.13 | |
| Fe2O3 | % m/m | 12.26 | 13.17 | 4.31 | 12.33 | 11.66 | | 12.48 | 11.92 | 12.58 | | 12.48 | 12.52 | |
| Fe(II)O | % m/m | | 10.5 | | | | | | | | | 8 | | |
| MnO | % m/m | 0.141 | 0.154 | 0.14 | 0.15 | 0.139 | | 0.15 | 0.14 | 0.141 | 0.153 | 0.13 | 0.14 | |
| MgO | % m/m | 4.38 | 4.09 | 12.34 | 4.42 | 4.048 | | 4.45 | 4.16 | 4.31 | | 4.11 | 4 | |
| CaO | % m/m | 6.99 | 6.93 | 6.93 | 6.84 | 6.807 | | 7.07 | 6.63 | 6.82 | | 6.71 | 6 | |
| Na2O | % m/m | 2.64 | 3 | 2.64 | 2.64 | 2.790 | | 2.64 | 2.51 | 2.76 | 2.59 | 2.57 | 2.68 | |
| K2O | % m/m | 1.66 | 1.77 | 1.72 | 1.69 | 1.635 | | 1.65 | 1.57 | 1.65 | | 1.59 | 1.79 | |
| P2O5 | % m/m | 0.18 | 0.17 | 0.16 | 0.16 | 0.171 | | 0.18 | 0.19 | 0.174 | | 0.15 | | |
| H2O+ | % m/m | | | | | | | | | | | | | |
| CO2 | % m/m | | | | | 1.100 | | | | 0.66 | 0.698 | 0.64 | | |
| LOI | % m/m | 1.63 | 2.5 | | | 1.420 | | 1.77 | 1.68 | 1.48 | | 1.53 | | |
| Ag | mg kg-1 | 0.698 | 0.8688 | | | | | | | 1.41 | | | | |
| As | mg kg-1 | | | | | | | 1.58 | | 2.48 | 2.21 | 3 | | 1.8 |
| Au | mg kg-1 | 0.042 | 0.2646 | | | | | | | 0.0317 | 0.0415 | | | |
| B | mg kg-1 | | 5.5056 | | | | | | | | | 17 | | |
| Ba | mg kg-1 | 499 | 461.751 | | | | | 474 | 430 | 454 | 422 | 463 | 450 | |
| Be | mg kg-1 | 1.262 | 1.11345 | | | | | 1.21 | | | | 1.6 | | |
| Bi | mg kg-1 | 0.879 | 0.6893 | | | | | 1.14 | | 0.91 | | | | |
| Br | mg kg-1 | | | | | | | | | | | | | |
| Cd | mg kg-1 | 0.38 | 0.43655 | | | | | 0.48 | | 0.42 | | | | |
| Ce | mg kg-1 | 55.04 | 63.4571 | | | | | 57.3 | | 54.1 | 69 | 50 | 60.3 | |
| Cl | mg kg-1 | | | | | | | | | 496 | 399 | | 490 | |
| Co | mg kg-1 | 83.4 | 78.5597 | | | | | 77.4 | 63 | 80.6 | 74 | 78 | 82.9 | |
| Cr | mg kg-1 | 166 | 145.214 | 41 | | | | 154 | 147 | 158 | 152 | 153 | 162 | |
| Cs | mg kg-1 | 4.462 | 4.6946 | | | | | 4.06 | | 4.46 | 3.9 | | 4.2 | |
| Cu | mg kg-1 | 962 | 1285.21 | 876 | | | | 1070 | 848 | 1341 | | | 1280 | |
| Dy | mg kg-1 | 4.71 | 4.5903 | | | | | 4.47 | | 4.37 | 4.32 | 2.3 | 4.5 | |
| Er | mg kg-1 | 2.79 | 2.72465 | | | | | 2.63 | | 2.69 | | 1.3 | | |
| Eu | mg kg-1 | 1.271 | 1.22135 | | | | | 1.29 | | 1.25 | 1.34 | 0.75 | 1.4 | |
| F | mg kg-1 | | | | | | | | | | | | | |
| Ga | mg kg-1 | 18.13 | 19.2268 | | | | | 19.5 | 14 | 18.9 | | 20 | | 19 |
| Gd | mg kg-1 | 4.831 | 4.76345 | | | | | 4.63 | | 4.66 | | 2.8 | | |
| Ge | mg kg-1 | | 1.40295 | | | | | 1.26 | | | | | | |
| Hf | mg kg-1 | 4.383 | 4.3266 | | | | | 4.38 | | 4.45 | 4.34 | 5.6 | 4.88 | |
| Hg | mg kg-1 | | | | | | | | | | | | | |
| Ho | mg kg-1 | 0.972 | 0.97385 | | | | | 0.904 | | 0.88 | 1 | 0.4 | | |
| I | mg kg-1 | | | | | | | | | | | | | |
| In | mg kg-1 | | | | | | | 0.12 | | | 0.1 | | | |
| Ir | mg kg-1 | | 0.03535 | | | | | | | 0.00661 | 0.006 | | | |
| La | mg kg-1 | 27.57 | 24.1925 | | | | | 27.9 | | 26.6 | 26.3 | 28 | 28.2 | |
| Li | mg kg-1 | 35.84 | 31.0415 | | | | | | | | | 35 | | |
| Lu | mg kg-1 | 0.436 | 0.43005 | | | | | 0.438 | | 0.43 | 0.4 | 0.14 | 0.46 | |
| Mo | mg kg-1 | 1.753 | 1.42545 | | | | | 1.69 | | 3.26 | | | | |
| N | mg kg-1 | | | | | | | | | | | | | |
| Nb | mg kg-1 | 8.85 | 8.6278 | 8 | | | | 7.55 | 9 | 8.17 | | 8.8 | | |
| Nd | mg kg-1 | 25.91 | 24.7057 | | | | | 24.7 | | 24.7 | 23.4 | 16.8 | 32 | |
| Ni | mg kg-1 | 876 | 1244.09 | 908 | | | | 1175 | 743 | 1242 | 1186 | | 1120 | |
| Os | mg kg-1 | | | | | | | | | 0.00631 | 0.0035 | | | |
| Pb | mg kg-1 | 82.8 | 92.2004 | | | | | 85.6 | 72 | 77.9 | | 77 | | |
| Pd | mg kg-1 | 0.133 | 6.2362 | | | | | | | 0.104 | 0.1839 | | | |
| Pr | mg kg-1 | 6.557 | 6.31615 | | | | | 6.66 | | 6.19 | | 5 | | |
| Pt | mg kg-1 | 0.083 | 0.05235 | | | | | | | 0.0728 | 0.1505 | | | |
| Rb | mg kg-1 | 61.3 | 62.2473 | 62 | | | | 60.4 | 56 | 61.6 | 63.2 | 59 | 66 | |
| Re | mg kg-1 | | 0.0077 | | | | | | | | 0.0047 | | | |
| Rh | mg kg-1 | | 0.0395 | | | | | | | 0.017 | 0.0166 | | | |
| Ru | mg kg-1 | | 0.01865 | | | | | | | 0.0165 | 0.0108 | | | |
| S | mg kg-1 | 10800 | | | | | 11000 | 10600 | | 10900 | 10338 | 11017 | | |
| Sb | mg kg-1 | 10.6 | 11.3291 | | | | | | | 10.4 | 9.06 | 10.1 | 8 | 9.7 |
| Sc | mg kg-1 | 22.8 | 19.9795 | | | | | | | 23 | 25.3 | 24.2 | 24 | 25.6 |
| Se | mg kg-1 | | | | | | | | | | 3.36 | | | 3.5 |
| Sm | mg kg-1 | 5.105 | 4.84675 | | | | | 5.11 | | 4.53 | 4.7 | | 5.1 | |
| Sn | mg kg-1 | 18.6 | 21.0695 | | | | | 19.4 | | 20.4 | | 17 | | |
| Sr | mg kg-1 | 270 | 267.883 | 252 | | | | 253 | 233 | 272 | 235 | 258 | | 320 |
| Ta | mg kg-1 | 0.564 | 1.6943 | | | | | 0.69 | | 0.6 | 0.51 | | | 0.51 |
| Tb | mg kg-1 | 0.777 | 0.72145 | | | | | 0.723 | | 0.82 | 0.7 | 0.34 | 0.77 | |
| Te | mg kg-1 | 0.38 | 0.28775 | | | | | | | | | | | |
| Th | mg kg-1 | 7.19 | 7.14725 | 6 | | | | 7.33 | 8 | 7.4 | 7.2 | | 7 | |
| Tl | mg kg-1 | 0.51 | 0.57875 | | | | | | | 0.51 | | | | |
| Tm | mg kg-1 | 0.428 | 0.421 | | | | | 0.403 | | 0.39 | | | | |
| U | mg kg-1 | 1.687 | 2.1265 | 3 | | | | 1.87 | | 1.6 | 1.6 | | | 1.7 |
| V | mg kg-1 | 203.6 | 203.861 | | | | | 187 | 179 | 190 | 223 | 198 | 208 | |
| W | mg kg-1 | 1.16 | 1.0245 | | | | | 1.07 | | 1.19 | | | | |
| Y | mg kg-1 | 25.5 | 24.43 | 26 | | | | 25.7 | 24 | 25.9 | | 26 | | |
| Yb | mg kg-1 | 2.78 | 2.74 | | | | | 2.78 | | 2.34 | 2.6 | 0.96 | 2.86 | |
| Zn | mg kg-1 | 122 | 115.18 | 120 | | | | 129 | 109 | 136 | 83 | 119 | | 70 |
| Zr | mg kg-1 | 163.4 | 163.91 | 150 | | | | 168 | 148 | 170 | 43 | 146 | | 210 |

| Table 1 | | GeoPT18 Analytical results submitted (Dec. 2005) | | | | | | | | | | | |
|------------------|---------|--|-------|---------|-------|-------|-------|--------|-------|-------|-------|-------|-------|
| | | Quartz diorite KPT-1 | | | | | | | | | | | |
| Round identifier | | S45 | S46 | S47 | S48 | S49 | S50 | S51 | S52 | S53 | S54 | S55 | S56 |
| Sample | | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Data quality | | 1 | 2 | 2 | 1 | 2 | 2 | 2 | 2 | 1 | 2 | 1 | 2 |
| SiO2 | % m/m | 53.811 | 54.6 | 53.16 | 52.55 | 53.56 | 54.9 | 53.712 | 54.75 | | 56.5 | 54.15 | |
| TiO2 | % m/m | 0.8962 | 0.93 | 0.9 | 0.95 | 0.9 | 0.89 | 0.941 | 0.907 | 0.97 | 0.86 | 0.908 | 0.95 |
| Al2O3 | % m/m | 14.365 | 14.80 | 14.14 | 13.61 | 14.28 | 14.7 | 14.2 | 14.69 | 14.9 | 13.1 | 14.37 | 15.07 |
| Fe2O3 | % m/m | 12.324 | 12.40 | 12.26 | 11.47 | 12.1 | 12.2 | 12.364 | 12.27 | 12.2 | 11.2 | 12.31 | 12.09 |
| Fe(II)O | % m/m | | 8.54 | 7.47 | 7.51 | | | 8.249 | | | | | |
| MnO | % m/m | 0.1449 | 0.148 | 0.13 | 0.14 | 0.14 | 0.14 | 0.149 | 0.147 | 0.14 | 0.11 | 0.15 | 0.16 |
| MgO | % m/m | 4.326 | 4.45 | 4.43 | 4.19 | 4.14 | 4.38 | 4.697 | 4.13 | 4.3 | 3.55 | 4.21 | |
| CaO | % m/m | 6.864 | 6.8 | 7.3 | 6.88 | 6.82 | 6.89 | 7.358 | 6.91 | 6.6 | 6.02 | 6.9 | |
| Na2O | % m/m | 2.631 | 2.60 | 2.41 | 2.87 | 2.55 | 2.67 | 2.59 | 2.63 | 2.8 | 4.04 | 2.56 | 14.07 |
| K2O | % m/m | 1.650 | 1.65 | 1.68 | 1.6 | 1.63 | 1.65 | 1.64 | 1.65 | 1.8 | 1.85 | 1.61 | 19.83 |
| P2O5 | % m/m | 0.1632 | 0.17 | 0.13 | 0.16 | 0.16 | 0.16 | 0.158 | 0.172 | 0.16 | 0.1 | 0.167 | |
| H2O+ | % m/m | 0.053 | | | 1.64 | | | | | | | | |
| CO2 | % m/m | | 0.75 | | 0.69 | | | | | 0.37 | | | |
| LOI | % m/m | 1.256 | 1.50 | 1.57 | 1.63 | 1.74 | 1.47 | 2.075 | 1.54 | | 1.4 | 1.32 | |
| Ag | mg kg-1 | | 0.6 | | | | | | | 0.7 | | | 1 |
| As | mg kg-1 | | 2 | | 5 | | | | | 2.8 | 7 | | |
| Au | mg kg-1 | | 0.031 | 0.04 | | | | | | | | | 1 |
| B | mg kg-1 | | | | | | | | | | | | |
| Ba | mg kg-1 | 458.6 | 465 | | 468 | 459.2 | 435 | 510.12 | | 500 | | 643 | |
| Be | mg kg-1 | | 1.3 | | | | | | | 1.4 | | | |
| Bi | mg kg-1 | | 0.92 | | 0 | | | | | | | | |
| Br | mg kg-1 | | | | | | | | | | | | |
| Cd | mg kg-1 | | 0.45 | | 5 | | 0.5 | | | 0.1 | | | |
| Ce | mg kg-1 | 51.778 | 56.5 | | 83 | 55.7 | 54.4 | 59.39 | | | | | |
| Cl | mg kg-1 | | | | 272 | | | 310 | | | | | |
| Co | mg kg-1 | | 82 | 50.46 | 80 | | 101 | 63 | | 81 | 60 | | |
| Cr | mg kg-1 | 151.3 | 165 | 140 | 220 | | 145 | 140 | | 150 | 162 | 165.3 | |
| Cs | mg kg-1 | 4.329 | 4.45 | | 1 | 4.5 | 4.3 | 4 | | | | | |
| Cu | mg kg-1 | | 1330 | 1170 | 1065 | | 1142 | 1200 | | 1300 | 867 | 865.3 | 1560 |
| Dy | mg kg-1 | 4.957 | 4.8 | | 2 | 4.389 | 4.5 | 4.08 | | | | | |
| Er | mg kg-1 | 2.767 | 2.7 | | 2 | 2.675 | 2.8 | 2.44 | | | | | |
| Eu | mg kg-1 | 1.304 | 1.25 | | 1 | 1.195 | 1.5 | 1.18 | | | | | |
| F | mg kg-1 | | 535 | | 754 | | | | | | | | |
| Ga | mg kg-1 | 17.6 | 19 | | 16 | | | 28.82 | | 25 | | 28.2 | |
| Gd | mg kg-1 | 4.796 | 4.65 | | 6 | 4.491 | 4.6 | 4.38 | | | | | |
| Ge | mg kg-1 | | 1.4 | | | | | 1.84 | | | | | |
| Hf | mg kg-1 | 4.597 | 4.4 | | 11 | 4.62 | | 3.39 | | | | | |
| Hg | mg kg-1 | | | | | | | | | 0.02 | | | |
| Ho | mg kg-1 | 1.017 | 0.93 | | 1 | 0.938 | 1.01 | 0.98 | | | | | |
| I | mg kg-1 | | | | | | | | | | | | |
| In | mg kg-1 | | 0.11 | | | | | | | | | | |
| Ir | mg kg-1 | | 0.008 | | | | | | | | | | |
| La | mg kg-1 | 27.058 | 27.5 | | 33 | 26.38 | 26.1 | 31 | | 28 | | | |
| Li | mg kg-1 | | 35 | | | | 43 | 30.9 | | 37 | | | |
| Lu | mg kg-1 | 0.424 | 0.41 | | | 0.409 | 0.42 | 0.4 | | | | | |
| Mo | mg kg-1 | | 1.5 | | 1 | | | | | 2 | | | |
| N | mg kg-1 | | | | | | | | | | | | |
| Nb | mg kg-1 | 8.382 | 8.5 | | 8 | 8.58 | | 12.79 | | | | 9.5 | |
| Nd | mg kg-1 | 23.051 | 25 | | 36 | 25.29 | 24.8 | 27 | | | | | |
| Ni | mg kg-1 | 1198.6 | 1250 | 1082.21 | 1002 | | 1152 | 620 | | 1100 | 729 | 540 | 1100 |
| Os | mg kg-1 | | 0.002 | | | | | | | | | | |
| Pb | mg kg-1 | 81.331 | 80 | | 75 | 83.1 | 76.1 | 59 | | 83 | 74 | 52.2 | 44 |
| Pd | mg kg-1 | | 0.155 | 0.18 | | | | | | | | | |
| Pr | mg kg-1 | 5.796 | 6.5 | | 10 | 6.467 | 6.5 | 7 | | | | | |
| Pt | mg kg-1 | | 0.09 | 0.06 | | | | | | | | | |
| Rb | mg kg-1 | 61.10 | 64.5 | | 60 | 66.8 | 65.8 | 54.5 | | | | 60.3 | |
| Re | mg kg-1 | | | | | | | | | | | | |
| Rh | mg kg-1 | | 0.018 | | | | | | | | | | |
| Ru | mg kg-1 | | 0.018 | | | | | | | | | | |
| S | mg kg-1 | | 11500 | 10440 | 3880 | | | 5500 | 810 | 10600 | | | |
| Sb | mg kg-1 | | 11.1 | | 3 | | 10.8 | | | 11 | | | |
| Sc | mg kg-1 | 25.7 | 25 | | 37 | 27.5 | 27.2 | 25 | | | | | |
| Se | mg kg-1 | | 4 | | | | | | | 3.1 | | | |
| Sm | mg kg-1 | 5.146 | 4.8 | | 10 | 4.86 | 5.1 | 5.94 | | | | | |
| Sn | mg kg-1 | | 20 | | 6 | | | 30.8 | | 17 | | | |
| Sr | mg kg-1 | 254.2 | 265 | | 259 | 270.1 | 324 | 271.2 | | 280 | | 274.1 | |
| Ta | mg kg-1 | 0.631 | 0.7 | | 0 | 0.6 | | 0.81 | | | | | |
| Tb | mg kg-1 | 0.804 | 0.7 | | 3 | 0.731 | 0.71 | 0.78 | | | | | |
| Te | mg kg-1 | | 0.4 | | | | | | | | | | |
| Th | mg kg-1 | 7.363 | 6.9 | | 6 | 6.793 | 11.7 | 7.01 | | | | 4.6 | |
| Tl | mg kg-1 | | 0.55 | | | | | | | | | | |
| Tm | mg kg-1 | 0.411 | 0.41 | | | 0.406 | 0.4 | 0.39 | | | | | |
| U | mg kg-1 | 1.676 | 1.75 | | 2 | 1.684 | 1.8 | 1.71 | | | | | |
| V | mg kg-1 | 195.7 | 205 | 400 | 195 | | 175 | 200 | | 190 | | 246 | |
| W | mg kg-1 | | 1.4 | | 2 | | | | | | | | |
| Y | mg kg-1 | 27.378 | 26 | | 26 | 24.6 | 25 | 28.6 | | | | 35.2 | |
| Yb | mg kg-1 | 2.677 | 2.7 | | 2 | 2.673 | 2.7 | 2.2 | | | | | |
| Zn | mg kg-1 | 115.7 | 122 | 84.6 | 125 | | 126 | 93 | | 140 | 119 | 100.6 | 87 |
| Zr | mg kg-1 | 170.8 | 165 | | 157 | 180.7 | 182 | 127.5 | | | 156 | 140.7 | |

| Table 1 | | GeoPT18 Analytical results submitted (Dec. 2005) | | | | | | | | | | | | |
|------------------|---------|--|-------|-------|---------|-------|-------|-------|-------|-------|-------|--------|-------|-------|
| | | Quartz diorite KPT-1 | | | | | | | | | | | | |
| Round identifier | | S57 | S58 | S59 | S60 | S61 | S62 | S63 | S64 | S65 | S66 | S67 | S68 | S68 |
| Sample | | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Data quality | | 2 | 2 | 1 | 1 | 1 | 1 | 1 | 1 | 1 | 2 | 2 | 1 | 2 |
| SiO2 | % m/m | 54.36 | 54.52 | 54.40 | 54.208 | 54.16 | | 49.5 | | | 54 | 53.68 | 53.38 | |
| TiO2 | % m/m | 0.926 | 0.91 | 0.91 | 0.897 | 0.94 | 0.89 | 0.852 | | | 0.966 | 0.88 | 0.909 | |
| Al2O3 | % m/m | 14.67 | 14.46 | 14.53 | 14.425 | 15.14 | | 12.61 | | | 14.6 | 14.36 | 14.24 | |
| Fe2O3 | % m/m | 12.33 | 12.3 | 12.38 | 12.2 | 12.36 | | 12.83 | | 12.22 | 12.9 | 12.020 | 12.23 | |
| Fe(II)O | % m/m | | | | | | | | | | | | | |
| MnO | % m/m | 0.149 | 0.15 | 0.14 | 0.146 | 0.16 | 0.13 | 0.141 | | | 0.14 | 0.149 | 0.149 | |
| MgO | % m/m | 4.361 | 4.3 | 4.27 | 4.348 | | | 3.97 | | | 4.41 | 4.26 | 4.36 | |
| CaO | % m/m | 7.067 | 6.66 | 7.03 | 6.889 | 6.85 | | 6.23 | | | 7.05 | 6.820 | 6.98 | |
| Na2O | % m/m | 2.581 | 2.55 | 2.44 | 2.575 | 2.43 | 2.68 | | | | 2.56 | 2.62 | 2.57 | |
| K2O | % m/m | 1.615 | 1.66 | 1.65 | 1.646 | 1.94 | 1.74 | 1.6 | | | 1.71 | 1.63 | 1.65 | |
| P2O5 | % m/m | 0.169 | 0.17 | 0.17 | 0.193 | 0.18 | 0.17 | | | | 0.138 | 0.16 | 0.168 | |
| H2O+ | % m/m | | | | | | | | | | | | 2.05 | |
| CO2 | % m/m | | | | 0.666 | | | 0.696 | | | | | 0.62 | |
| LOI | % m/m | | 1.62 | 1.28 | 1.403 | 1.73 | 1.63 | 1.67 | | | 1.3 | 2.11 | 1.49 | |
| Ag | mg kg-1 | | | | | | | | | | | 0.93 | | |
| As | mg kg-1 | | | 3.3 | 2.007 | | | | | | | 1.7 | | |
| Au | mg kg-1 | | 0.059 | | | | | | | | 0.031 | | | |
| B | mg kg-1 | | | | | | | | | | | | | |
| Ba | mg kg-1 | 465.4 | 523 | 468 | 471.33 | 488 | 509 | | 457.3 | 434 | 577 | 523.1 | 466 | |
| Be | mg kg-1 | 1.6 | | | 1.447 | | | | | | 1.73 | 1.34 | | |
| Bi | mg kg-1 | | | | 0.847 | | | | | | | 2.3 | | |
| Br | mg kg-1 | | | | | | | | | | | | | |
| Cd | mg kg-1 | | | | 0.398 | | | | | | 0.35 | 0.353 | | |
| Ce | mg kg-1 | 56.04 | 43 | 51.23 | 55.733 | 62 | 53 | | 52.75 | 54.5 | 55.87 | 54.37 | 55.7 | |
| Cl | mg kg-1 | | | | | | | | | | | | | 492 |
| Co | mg kg-1 | 82.84 | | 81.3 | 82.6 | 60 | 57 | | | 78.4 | 76.1 | 79.3 | 73 | |
| Cr | mg kg-1 | 151.3 | 161 | 159.2 | 179 | 166 | 137 | | | | 172 | 155 | 154 | |
| Cs | mg kg-1 | 4.6 | | | 4.54 | | | | 4.42 | 4.0 | 4.57 | 4.383 | 4.36 | |
| Cu | mg kg-1 | 1054 | 936 | 1431 | 1377 | 933 | 601 | | | | 1158 | 1232 | 1064 | |
| Dy | mg kg-1 | 4.61 | | 4.07 | 5.157 | | | | 4.25 | | 4.45 | 4.55 | 4.40 | |
| Er | mg kg-1 | 2.86 | | 2.51 | 2.7 | | | | 2.54 | | 2.82 | 2.71 | 2.70 | |
| Eu | mg kg-1 | 1.36 | | 1.21 | 1.253 | | | | 1.12 | 1.28 | 1.27 | 1.255 | 1.19 | |
| F | mg kg-1 | | | | | | 700 | | | | | | | 392 |
| Ga | mg kg-1 | 18.38 | 17 | 19.4 | 18.333 | 15 | | | | | 18.03 | 18.2 | 18 | |
| Gd | mg kg-1 | 4.59 | | 4.43 | 4.77 | | | | 4.25 | | 4.58 | 4.53 | 4.26 | |
| Ge | mg kg-1 | | | | | | | | | | 1.34 | 1.8 | | |
| Hf | mg kg-1 | 4.56 | 10 | | 4.353 | | | | | 4.6 | 4.35 | 3.7 | 4.06 | |
| Hg | mg kg-1 | | | | | | | | | | | | | |
| Ho | mg kg-1 | 1.04 | | 0.83 | 1.013 | | | | 0.872 | | 0.917 | 0.966 | 0.97 | |
| I | mg kg-1 | | | | | | | | | | | | | |
| In | mg kg-1 | | | | | | | | | | | | | |
| Ir | mg kg-1 | | | | | | | | | | | | | |
| La | mg kg-1 | 27.58 | 32 | 24.05 | 28.633 | 24 | | | 25.1 | 26.9 | 26.83 | 26.08 | 23.9 | |
| Li | mg kg-1 | | | | 42.967 | | | | | | | 33.21 | | |
| Lu | mg kg-1 | 0.42 | | 0.36 | 0.441 | | | | 0.4 | 0.36 | 0.397 | 0.415 | 0.42 | |
| Mo | mg kg-1 | | | | | | | | | | 2.28 | 1.7 | | |
| N | mg kg-1 | | | | | | | | | | | | | |
| Nb | mg kg-1 | 8.23 | 7 | | 7.1 | 11 | | | 7.97 | | 10.26 | 7.3 | 7.59 | |
| Nd | mg kg-1 | 25.35 | 27 | 22.49 | 24.167 | | | | 23.8 | 28 | 24.47 | 25.02 | 24.9 | |
| Ni | mg kg-1 | 1089 | 870 | 1197 | 1335 | 872 | 773 | | | | 1013 | 1188 | 988 | |
| Os | mg kg-1 | | | | | | | | | | | | | |
| Pb | mg kg-1 | | 80 | 101.0 | 81.133 | 81 | 68 | | 76.5 | | 76.8 | 82.9 | 81.9 | |
| Pd | mg kg-1 | | | | | | | | | | 0.145 | | | |
| Pr | mg kg-1 | 6.55 | | 6.08 | 5.98 | | | | 5.87 | | 6.497 | 6.37 | 6.50 | |
| Pt | mg kg-1 | | | | | | | | | | 0.06 | | | |
| Rb | mg kg-1 | 65.24 | 60 | 65.5 | 61.233 | 69 | 48 | | 59 | 55.5 | 62.1 | 59.9 | 57.7 | |
| Re | mg kg-1 | | | | | | | | | | | | | |
| Rh | mg kg-1 | | | | | | | | | | | | | |
| Ru | mg kg-1 | | | | | | | | | | | | | |
| S | mg kg-1 | | 10300 | | | | 12300 | 10500 | | | 8400 | | 929 | |
| Sb | mg kg-1 | | | | 10.767 | | | | | | 9.41 | 9.8 | | |
| Sc | mg kg-1 | 24.4 | | 27.2 | 25.533 | 24 | 26 | | | 24.7 | | 24.9 | 23.8 | |
| Se | mg kg-1 | | | | 2.527 | | | | | | 2.92 | 2.5 | | |
| Sm | mg kg-1 | 5.18 | | 4.54 | 5.317 | | | | 4.52 | 4.9 | 4.96 | 4.64 | 4.97 | |
| Sn | mg kg-1 | | 17 | | 20.6 | | | | | | 18.9 | 18.9 | | |
| Sr | mg kg-1 | 303.5 | 256 | 258.6 | 274.6 | 264 | 243 | | 253.8 | | 277 | 256.3 | 259 | |
| Ta | mg kg-1 | 0.64 | | | 0.64 | | | | 0.52 | 0.47 | 0.567 | | 0.25 | |
| Tb | mg kg-1 | 0.76 | | 0.69 | 0.78 | | | | 0.668 | 0.85 | 0.74 | 0.737 | 0.67 | |
| Te | mg kg-1 | | | | | | | | | | | | | |
| Th | mg kg-1 | 7.25 | 8 | 6.04 | 7.37 | | 3 | | 7.5 | 7.3 | 11.57 | 7.373 | 6.89 | |
| Tl | mg kg-1 | | | | 0.544 | | | | | | | 0.223 | | |
| Tm | mg kg-1 | 0.43 | | 0.37 | 0.441 | | | | 0.382 | | 0.4 | 0.418 | 0.42 | |
| U | mg kg-1 | 1.83 | | 1.88 | 1.717 | | | | 1.76 | 1.68 | | 1.775 | 1.66 | |
| V | mg kg-1 | 182.5 | 202 | 180.8 | 205.667 | 221 | 193 | | | | 172 | 195.6 | 202 | |
| W | mg kg-1 | 1.15 | | | | | | | | | | 0.97 | | |
| Y | mg kg-1 | 27.9 | 25 | 25.0 | 26.4 | 35 | 8 | | 25.9 | | 23.6 | 25.7 | 25.8 | |
| Yb | mg kg-1 | 2.73 | | 2.43 | 2.89 | | | | 2.31 | 2.9 | 2.64 | 2.64 | 2.62 | |
| Zn | mg kg-1 | 130.7 | 113 | 118.3 | 125.333 | 106 | 108 | | | 118 | 134.6 | 122.9 | 120 | |
| Zr | mg kg-1 | 169.1 | 167 | 166 | 156.067 | 157 | 120 | | | | 159 | 162.7 | 164 | |

| Table 1 | | GeoPT18 Analytical results submitted (Dec. 2005) | | | | | | | | | Data not received | |
|------------------|---------|--|-------|-------|-------|-------|-------|-------|-------|-------|-------------------|--------|
| | | Quartz diorite KPT-1 | | | | | | | | | | |
| Round identifier | | S69 | S70 | S71 | S72 | S73 | S74 | S75 | S76 | S77 | S78 | S79 |
| Sample | | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Data quality | | 2 | 2 | 2 | 1 | 2 | 2 | 2 | 1 | 1 | 1 | 1 |
| SiO2 | % m/m | 55.35 | 54.45 | 52.9 | | | 53.2 | 53.99 | 53.8 | 54.56 | 54.40 | 54.20 |
| TiO2 | % m/m | 0.86 | 0.88 | 0.9 | | 0.86 | 0.89 | 0.905 | 0.85 | 0.92 | 0.90 | 0.967 |
| Al2O3 | % m/m | 14.2 | 14.31 | 14.1 | | | 14 | 15.03 | 14.5 | 15.34 | 14.70 | 13.87 |
| Fe2O3 | % m/m | 12.2 | 12.54 | 12 | | 12.15 | 12.2 | 12.53 | 11.97 | 11.9 | 12.60 | 12.55 |
| Fe(II)O | % m/m | | | 9.4 | | | | | | | | |
| MnO | % m/m | 0.15 | 0.14 | 0.14 | | 0.15 | 0.13 | 0.145 | 0.135 | 0.18 | 0.15 | 0.128 |
| MgO | % m/m | 4.31 | 4.24 | 4.31 | | | 4.4 | 4.47 | 4.3 | 3.73 | 3.73 | 3.78 |
| CaO | % m/m | 6.77 | 6.9 | 7.06 | | 6.78 | 6.8 | 6.95 | 6.79 | 7.15 | 7.15 | 6.87 |
| Na2O | % m/m | 2.64 | 2.64 | 2.6 | | | 2.4 | 2.78 | 2.57 | 2.27 | 2.76 | 2.68 |
| K2O | % m/m | 1.64 | 1.68 | 1.63 | | 1.94 | 1.6 | 1.58 | 1.56 | 1.7 | 1.76 | 1.74 |
| P2O5 | % m/m | 0.15 | 0.16 | 0.16 | | | 0.21 | 0.17 | 0.17 | 0.21 | 0.21 | 0.233 |
| H2O+ | % m/m | 1.26 | | 1.8 | | | | | | | | |
| CO2 | % m/m | 0.55 | | | | | 0.59 | | | | | |
| LOI | % m/m | 1.43 | 1.14 | 1.25 | 1.51 | | 1.51 | | | 1.29 | 1.41 | 1.56 |
| Ag | mg kg-1 | | | | | | | | | 20 | | |
| As | mg kg-1 | | | 2.2 | | | | | | | | 0.0014 |
| Au | mg kg-1 | 0.034 | | | | | | | | | | |
| B | mg kg-1 | | | | | | | | | 28 | | |
| Ba | mg kg-1 | 456.5 | 530 | 440 | 477 | | 467 | 306 | | 509 | | 0.0443 |
| Be | mg kg-1 | 1.39 | | 1.6 | | | | | | | | |
| Bi | mg kg-1 | | | 1.07 | | | | | | | | |
| Br | mg kg-1 | | | | | | | | | | | |
| Cd | mg kg-1 | 0.175 | | 0.4 | | | | | | 3 | | |
| Ce | mg kg-1 | 54.08 | | 52.2 | 44 | | 65 | 54.26 | | 39 | | |
| Cl | mg kg-1 | | | 440 | | | 540 | | | | | |
| Co | mg kg-1 | 77.87 | 95 | 77.4 | 77 | | 76 | 51 | | 70 | | 0.0051 |
| Cr | mg kg-1 | 149.91 | 145 | 135 | 161 | 110 | 126 | 107 | | 165 | | 0.0093 |
| Cs | mg kg-1 | 4.298 | | 4.2 | | | | | | | | |
| Cu | mg kg-1 | 1140 | 1490 | 1210 | 892 | 1075 | 1584 | 988 | | 1191 | | 0.113 |
| Dy | mg kg-1 | 4.502 | | 4.52 | | | | 4.5 | | 3 | | |
| Er | mg kg-1 | 2.74 | | 3.05 | | | | 2.67 | | 12.9 | | |
| Eu | mg kg-1 | 1.19 | | 1.2 | | | | 1.27 | | 0.6 | | |
| F | mg kg-1 | | | 460 | | | 250 | | | | | |
| Ga | mg kg-1 | 18.23 | | 18 | 19 | 13 | | 16 | | | | |
| Gd | mg kg-1 | 4.51 | | 4.67 | | | | 4.5 | | 14.9 | | |
| Ge | mg kg-1 | | | | | | | | | | | |
| Hf | mg kg-1 | 4 | | 4 | | | | | | | | |
| Hg | mg kg-1 | | | | | | | | | | | |
| Ho | mg kg-1 | 0.93 | | 0.89 | | | | 0.93 | | | | |
| I | mg kg-1 | | | | | | | | | | | |
| In | mg kg-1 | | | 0.11 | | | | | | | | |
| Ir | mg kg-1 | 0.0067 | | | | | | | | | | |
| La | mg kg-1 | 26.32 | | 27.2 | 28 | | 27 | 25.58 | | 20 | | |
| Li | mg kg-1 | 37.35 | | 30 | | | 40 | | | 27 | | |
| Lu | mg kg-1 | 0.403 | | 0.44 | | | | 0.41 | | | | |
| Mo | mg kg-1 | 1.97 | | | | | | | | | | |
| N | mg kg-1 | | | | | | | | | | | |
| Nb | mg kg-1 | 8.30 | | 9 | 9 | | | | | 76 | | 0.0004 |
| Nd | mg kg-1 | 24.48 | | 24.5 | | | | 25.28 | | 20 | | |
| Ni | mg kg-1 | 1193 | 1270 | 1060 | 982 | 895 | 974 | 866 | | 1187 | | 0.073 |
| Os | mg kg-1 | | | | | | | | | | | |
| Pb | mg kg-1 | 80.9 | 85 | 88 | 72 | | 89 | 76 | | 373 | | 0.0069 |
| Pd | mg kg-1 | 0.103 | | | | | | | | | | |
| Pr | mg kg-1 | 6.32 | | 6.28 | | | | 6.34 | | | | |
| Pt | mg kg-1 | 0.151 | | | | | | | | | | |
| Rb | mg kg-1 | 60.88 | | 64.3 | 63 | 64 | | 64 | | | | |
| Re | mg kg-1 | | | | | | | | | | | |
| Rh | mg kg-1 | 0.0167 | | | | | | | | | | |
| Ru | mg kg-1 | 0.0162 | | | | | | | | | | |
| S | mg kg-1 | 10400 | | 1.03 | | | 10000 | | | 4800 | | 0.32 |
| Sb | mg kg-1 | 10.30 | | 11.4 | | | | | | | | |
| Sc | mg kg-1 | 24.58 | | 26.9 | 25 | | | 22.7 | | 40 | | |
| Se | mg kg-1 | 2.26 | | | | | | | | | | |
| Sm | mg kg-1 | 4.87 | | 4.9 | | | | 4.82 | | 1 | | |
| Sn | mg kg-1 | 19.48 | | 20.5 | | | | | | | | |
| Sr | mg kg-1 | 252.80 | | 272 | 271 | 270 | 230 | 253 | | 224 | | 0.033 |
| Ta | mg kg-1 | 0.54 | | | | | | | | 19 | | |
| Tb | mg kg-1 | 0.72 | | 0.76 | | | | 0.7 | | | | |
| Te | mg kg-1 | 0.244 | | 0.48 | | | | | | | | |
| Th | mg kg-1 | 6.85 | | 7.9 | 8 | | | 5.7 | | | | |
| Tl | mg kg-1 | 0.57 | | 0.58 | | | | | | | | |
| Tm | mg kg-1 | 0.403 | | 0.39 | | | | 0.39 | | | | |
| U | mg kg-1 | 1.669 | | 1.76 | 3 | | | | | | | |
| V | mg kg-1 | 191.84 | | 202 | 204 | | 169 | 145 | | | | 0.0191 |
| W | mg kg-1 | 1.04 | | | | | 14 | | | | | |
| Y | mg kg-1 | 24.47 | | 26 | 26 | 23 | 23 | 22.7 | | 23 | | 0.0024 |
| Yb | mg kg-1 | 2.68 | | 2.8 | | | | 2.66 | | 2.7 | | |
| Zn | mg kg-1 | 107.43 | 130 | 121 | 122 | 121 | 139 | 124 | | 94 | | 0.0185 |
| Zr | mg kg-1 | 156.2 | | 158 | 154 | 150 | 154 | 154 | | | | 0.0185 |

Table 2 GeoPT18 Assigned values and robust statistical analysis of contributed data

| (Quartz diorite, KPT-1) | | | | | | | | | | | |
|----------------------------------|----------------------|----------------------|------------|--------------------------|---------------|----|----------------------|----------------------|------------|--------------------------|---------------|
| | X_a | H_a | sdm | sdm/H_a | status | | X_a | H_a | sdm | sdm/H_a | status |
| | % m/m | % m/m | % m/m | | | | mg/kg | mg/kg | mg/kg | | |
| SiO ₂ | 54.14 | 0.594 | 0.102 | 0.173 | Assigned | Li | 35.10 | 1.643 | 1.306 | 0.795 | Assigned |
| TiO ₂ | 0.90 | 0.018 | 0.004 | 0.236 | Assigned | Lu | 0.42 | 0.038 | 0.005 | 0.135 | Assigned |
| Al ₂ O ₃ | 14.41 | 0.193 | 0.048 | 0.246 | Assigned | Mo | 1.72 | 0.127 | 0.118 | 0.928 | Assigned |
| Fe ₂ O ₃ T | 12.24 | 0.168 | 0.034 | 0.201 | Assigned | Nb | 8.48 | 0.492 | 0.153 | 0.310 | Assigned |
| MnO | 0.14 | 0.004 | 0.001 | 0.264 | Assigned | Nd | 24.64 | 1.217 | 0.239 | 0.197 | Assigned |
| MgO | 4.30 | 0.069 | 0.020 | 0.290 | Assigned | Pb | 81.07 | 3.346 | 0.994 | 0.297 | Assigned |
| CaO | 6.89 | 0.103 | 0.019 | 0.188 | Assigned | Pr | 6.39 | 0.387 | 0.056 | 0.144 | Assigned |
| Na ₂ O | 2.61 | 0.045 | 0.016 | 0.357 | Assigned | Rb | 61.45 | 2.645 | 0.582 | 0.220 | Assigned |
| K ₂ O | 1.65 | 0.031 | 0.005 | 0.178 | Assigned | Sb | 10.01 | 0.566 | 0.330 | 0.583 | Assigned |
| P ₂ O ₅ | 0.17 | 0.004 | 0.002 | 0.379 | Assigned | Sc | 24.84 | 1.225 | 0.295 | 0.241 | Assigned |
| | mg/kg | mg/kg | mg/kg | | | Se | 2.93 | 0.199 | 0.235 | 1.179 | Assigned |
| Ba | 465.27 | 14.764 | 2.165 | 0.147 | Assigned | Sm | 4.90 | 0.309 | 0.049 | 0.160 | Assigned |
| Be | 1.42 | 0.108 | 0.053 | 0.494 | Assigned | Sn | 19.13 | 0.982 | 0.384 | 0.391 | Assigned |
| Bi | 0.95 | 0.076 | 0.065 | 0.851 | Assigned | Sr | 261.04 | 9.036 | 2.230 | 0.247 | Assigned |
| Ce | 55.71 | 2.433 | 0.781 | 0.321 | Assigned | Ta | 0.60 | 0.052 | 0.019 | 0.364 | Assigned |
| Cr | 152.24 | 5.716 | 2.243 | 0.392 | Assigned | Tb | 0.74 | 0.062 | 0.010 | 0.166 | Assigned |
| Cs | 4.42 | 0.283 | 0.082 | 0.291 | Assigned | Th | 7.27 | 0.431 | 0.138 | 0.319 | Assigned |
| Dy | 4.47 | 0.285 | 0.054 | 0.188 | Assigned | Tl | 0.54 | 0.047 | 0.013 | 0.277 | Assigned |
| Er | 2.72 | 0.187 | 0.030 | 0.162 | Assigned | Tm | 0.41 | 0.037 | 0.004 | 0.114 | Assigned |
| Eu | 1.24 | 0.096 | 0.015 | 0.157 | Assigned | U | 1.76 | 0.129 | 0.023 | 0.175 | Assigned |
| Ga | 18.21 | 0.941 | 0.218 | 0.231 | Assigned | V | 197.22 | 7.121 | 1.815 | 0.255 | Assigned |
| Gd | 4.60 | 0.292 | 0.045 | 0.154 | Assigned | Y | 25.82 | 1.266 | 0.310 | 0.245 | Assigned |
| Hf | 4.41 | 0.282 | 0.084 | 0.297 | Assigned | Yb | 2.69 | 0.185 | 0.032 | 0.170 | Assigned |
| Ho | 0.95 | 0.077 | 0.012 | 0.158 | Assigned | Zn | 120.24 | 4.677 | 1.831 | 0.391 | Assigned |
| La | 26.91 | 1.311 | 0.321 | 0.245 | Assigned | Zr | 158.12 | 5.902 | 2.062 | 0.349 | Assigned |

| Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005) | | | | | | | | | | | | |
|---|-----------------------------|-------|-------|-------|-----------------------------|-------|-------|-------|-------|-------|-------|-------|
| | Quartz diorite KPT-1 | | | | Note: There is no S5 | | | | | | | |
| Identifier | S1 | S2 | S3 | S4 | S4 | S6 | S7 | S8 | S9 | S10 | S10 | S11 |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Quality | 2 | 2 | 2 | 1 | 2 | 2 | 2 | 1 | 2 | 1 | 2 | 1 |
| SiO2 | 0.2 | 0.4 | -2.6 | 0.7 | * | 0.2 | 0.2 | * | * | 0.4 | * | 2.4 |
| TiO2 | 0.3 | 0.9 | -1.0 | -0.4 | * | 0.3 | 0.1 | * | * | 0.5 | * | -6.5 |
| Al2O3 | 0.2 | 1.0 | -3.1 | 1.0 | * | 0.1 | 0.1 | * | * | 1.1 | * | -3.8 |
| Fe2O3 | 0.5 | 0.8 | -4.3 | 2.8 | * | 0.6 | -0.1 | * | -0.1 | -0.6 | * | -8.9 |
| MnO | 0.3 | 0.8 | -1.8 | 6.8 | * | 0.8 | 0.4 | * | * | 0.8 | * | -1.0 |
| MgO | 0.3 | 0.2 | -2.4 | -6.1 | * | -0.1 | 0.1 | * | * | 0.4 | * | 1.5 |
| CaO | 0.5 | 0.4 | -0.6 | 2.7 | * | -0.3 | 0.1 | * | * | -0.2 | * | -5.5 |
| Na2O | 0.3 | -1.0 | 1.4 | -10.5 | * | 0.5 | 0.0 | * | -0.7 | -0.8 | * | 4.3 |
| K2O | 0.0 | -0.2 | 2.8 | -6.2 | * | 0.3 | 0.1 | * | * | 0.3 | * | -0.3 |
| P2O5 | 0.5 | * | 2.8 | -8.3 | * | -0.7 | 0.1 | * | * | 0.7 | * | -1.4 |
| Ba | 0.1 | * | * | * | -3.4 | 1.9 | -0.3 | 0.0 | 0.1 | * | 0.8 | * |
| Be | * | * | * | * | * | * | * | -0.7 | * | * | * | * |
| Bi | * | * | * | * | * | * | * | * | * | * | * | * |
| Ce | 2.1 | * | * | * | -5.3 | * | 3.8 | -1.6 | 0.2 | * | * | * |
| Cr | -0.5 | * | * | * | -10.6 | -2.8 | -1.2 | -1.8 | -1.6 | * | 1.1 | * |
| Cs | * | * | * | * | 8.1 | * | * | 0.2 | 0.8 | * | * | * |
| Dy | * | * | * | * | * | * | * | -0.7 | * | * | * | * |
| Er | * | * | * | * | * | * | * | 0.6 | * | * | * | * |
| Eu | * | * | * | * | * | * | * | 0.0 | -0.4 | * | * | * |
| Ga | 0.4 | * | * | 0.8 | * | * | -0.3 | -0.7 | * | * | 0.3 | * |
| Gd | * | * | * | * | * | * | * | -0.7 | * | * | * | * |
| Hf | * | * | * | * | * | * | * | 0.9 | 1.5 | * | * | * |
| Ho | * | * | * | * | * | * | * | -0.8 | * | * | * | * |
| La | -0.7 | * | * | * | * | * | 9.1 | -1.4 | 0.0 | * | * | * |
| Li | * | * | * | * | * | * | * | -0.1 | * | * | * | * |
| Lu | * | * | * | * | * | * | * | 0.2 | 0.2 | * | * | * |
| Mo | * | * | * | 18.0 | * | * | * | -1.1 | * | * | * | * |
| Nb | 1.8 | * | * | 7.1 | * | * | 0.5 | -1.2 | * | 0.0 | * | * |
| Nd | -0.1 | * | * | * | * | * | * | -0.6 | 0.2 | * | * | * |
| Pb | -0.3 | * | * | 2.1 | * | 1.2 | 0.9 | -4.3 | * | 0.7 | * | * |
| Pr | * | * | * | * | * | * | * | -0.4 | * | * | * | * |
| Rb | 0.2 | * | -4.1 | 2.1 | * | * | 1.5 | 4.4 | 0.2 | 0.5 | * | * |
| Sb | * | * | * | * | * | * | * | 2.6 | -1.2 | * | * | * |
| Sc | * | * | * | * | -2.4 | * | -3.6 | -0.9 | 0.0 | * | -0.1 | * |
| Se | * | * | * | * | * | -2.3 | * | * | * | * | * | * |
| Sm | * | * | * | * | * | * | * | -0.3 | 0.3 | * | * | * |
| Sn | * | * | * | * | * | * | * | * | * | * | * | * |
| Sr | 0.2 | * | -4.2 | 1.2 | * | 1.4 | 0.3 | 0.1 | * | 0.9 | * | * |
| Ta | * | * | * | * | * | * | * | -0.2 | -0.3 | * | * | * |
| Tb | * | * | * | * | * | * | * | 0.3 | -0.6 | * | * | * |
| Th | * | * | * | 8.6 | * | -1.5 | 0.5 | -0.2 | 0.2 | * | * | * |
| Tl | * | * | * | * | * | * | * | -0.7 | * | * | * | * |
| Tm | * | * | * | * | * | * | * | -0.2 | * | * | * | * |
| U | * | * | * | 32.8 | * | * | -6.8 | -0.4 | 0.2 | * | * | * |
| V | -0.2 | * | * | * | -1.1 | * | -1.1 | -0.9 | * | * | 1.0 | * |
| Y | 0.3 | * | * | 3.3 | * | * | 1.8 | -1.3 | * | 0.3 | * | * |
| Yb | * | * | * | * | * | * | * | -0.2 | 0.3 | * | * | * |
| Zn | -0.1 | * | -3.2 | -1.1 | * | -0.2 | -3.3 | 2.3 | * | 0.9 | * | * |
| Zr | 0.6 | * | -3.2 | 0.8 | * | * | 36.7 | 3.4 | * | -1.6 | * | * |

| Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005) | | | | | | | | | | | | |
|---|-----------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|
| | Quartz diorite KPT-1 | | | | | | | | | | | |
| Identifier | S12 | S13 | S14 | S15 | S16 | S17 | S18 | S19 | S19 | S20 | S21 | S22 |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Quality | 2 | 2 | 2 | 1 | 1 | 2 | 1 | 1 | 2 | 2 | 2 | 1 |
| SiO2 | 0.6 | * | -0.1 | 0.5 | * | -5.3 | * | 1.8 | * | 1.0 | 0.2 | 0.1 |
| TiO2 | -0.9 | -1.0 | 0.4 | 1.3 | 10.8 | -1.6 | * | 5.6 | * | 0.1 | -0.2 | -0.4 |
| Al2O3 | -1.2 | -1.1 | 0.0 | 0.5 | 20.1 | 18.9 | * | -0.2 | * | 0.5 | 0.7 | 0.2 |
| Fe2O3 | -0.6 | -1.9 | 0.8 | -0.1 | 9.4 | -1.0 | * | 0.1 | * | -0.3 | 0.2 | 0.7 |
| MnO | 0.5 | 0.2 | 1.5 | -2.0 | 5.9 | 1.5 | * | -0.7 | * | -0.9 | -0.5 | -3.6 |
| MgO | -1.8 | 0.3 | -0.5 | 0.5 | 5.6 | * | * | -0.2 | * | 0.3 | 1.2 | 4.3 |
| CaO | 0.4 | 0.1 | 0.5 | -0.6 | 7.3 | 2.2 | * | 1.6 | * | -0.1 | 0.2 | 0.0 |
| Na2O | 2.1 | -0.4 | -1.8 | 0.8 | 4.8 | * | * | -4.2 | * | -1.1 | -0.7 | 2.8 |
| K2O | 0.5 | 1.5 | -0.2 | -0.4 | 77.6 | 4.6 | * | 0.7 | * | 0.2 | 0.2 | -4.2 |
| P2O5 | 1.2 | -0.1 | -0.2 | 2.3 | 18.3 | * | * | -6.4 | * | 0.6 | -1.8 | -8.3 |
| Ba | -0.1 | 0.0 | -0.9 | -0.6 | 9.7 | 0.3 | -0.5 | * | -0.4 | -0.9 | 0.5 | 0.3 |
| Be | * | * | * | * | * | * | * | -3.0 | * | * | -0.2 | * |
| Bi | 1.0 | -2.0 | * | * | * | * | * | * | 5.0 | * | * | * |
| Ce | -0.1 | -0.4 | -3.4 | -1.2 | * | -0.4 | -0.8 | * | 0.9 | * | 0.2 | 4.2 |
| Cr | 0.5 | -1.1 | -2.6 | -0.6 | 57.3 | 7.1 | 0.0 | * | 1.3 | * | 1.6 | 1.9 |
| Cs | 0.1 | -0.2 | -1.6 | -0.6 | 61.9 | * | -1.4 | * | * | * | 1.4 | * |
| Dy | 0.8 | -0.2 | * | 0.0 | * | * | 0.0 | -4.9 | * | * | * | * |
| Er | 0.8 | -0.2 | * | -0.1 | * | * | 0.2 | -5.8 | * | * | * | * |
| Eu | 0.5 | -0.2 | * | -0.4 | * | * | -0.7 | -1.8 | * | * | * | * |
| Ga | 0.5 | -0.2 | -0.6 | 0.4 | * | -0.6 | 0.8 | * | -0.1 | * | 1.9 | -2.4 |
| Gd | * | -0.4 | * | 0.1 | * | * | 1.0 | -3.0 | * | * | * | * |
| Hf | * | * | * | -0.2 | * | * | -1.4 | * | -2.3 | * | * | 1.0 |
| Ho | 0.8 | * | * | 0.0 | * | * | -0.1 | -5.0 | * | * | * | * |
| La | 0.0 | -0.3 | 0.8 | -0.5 | 10.7 | -1.1 | -1.6 | * | 0.8 | * | 0.7 | * |
| Li | * | * | * | * | 40.7 | * | * | -4.0 | * | * | * | * |
| Lu | 0.5 | -0.5 | * | 0.4 | 10.5 | * | -0.5 | -5.8 | * | * | * | * |
| Mo | 1.1 | -5.6 | -0.5 | * | 16.8 | * | * | * | 0.3 | * | 1.8 | * |
| Nb | -0.4 | * | -1.6 | 1.9 | * | -3.5 | -1.2 | * | -0.6 | * | * | 1.0 |
| Nd | 0.1 | -0.2 | -1.1 | -0.2 | * | -0.7 | -0.4 | * | -0.6 | * | * | -2.2 |
| Pb | 1.1 | 0.1 | -4.3 | -0.5 | 3.4 | 1.3 | * | * | 0.2 | * | * | * |
| Pr | 0.2 | -0.3 | * | 0.0 | * | * | -0.7 | 1.6 | * | * | * | 0.0 |
| Rb | 0.0 | -1.6 | 1.6 | 1.4 | * | -0.3 | -0.6 | * | -0.2 | * | 0.6 | 0.6 |
| Sb | 0.3 | 0.0 | -6.4 | * | 7.5 | * | * | -10.1 | * | * | 1.5 | * |
| Sc | -0.3 | -0.6 | 0.9 | 0.3 | 0.1 | * | * | * | 2.5 | * | * | -1.5 |
| Se | 2.2 | -0.6 | * | * | -2.2 | * | * | 11.9 | * | * | * | * |
| Sm | 0.0 | -0.1 | -3.1 | 0.1 | * | * | -0.5 | -1.2 | * | * | * | * |
| Sn | 0.4 | -0.2 | -0.6 | * | 10.1 | * | * | * | -0.5 | * | 0.3 | * |
| Sr | 0.3 | -5.1 | -0.9 | 0.2 | 0.5 | -0.1 | -0.2 | * | -0.2 | 2.7 | 0.6 | -2.3 |
| Ta | 0.0 | * | * | -0.8 | * | * | 0.2 | * | * | * | * | * |
| Tb | 0.6 | -0.4 | * | 0.4 | * | * | -0.2 | -3.4 | * | * | * | * |
| Th | * | -0.4 | 0.8 | -1.9 | 14.9 | * | -1.3 | * | 1.3 | * | 0.4 | * |
| Tl | 0.4 | -0.6 | * | * | * | * | * | * | * | * | -0.3 | * |
| Tm | 0.7 | * | * | 0.3 | * | * | -0.4 | -4.5 | * | * | * | * |
| U | 2.0 | -0.3 | 8.7 | -0.4 | 17.9 | * | -0.6 | * | 10.2 | * | 0.2 | * |
| V | 0.3 | -0.4 | -1.1 | -0.8 | 6.0 | 0.9 | 0.4 | * | 0.2 | * | 1.4 | 0.8 |
| Y | -0.7 | * | -0.7 | 1.7 | 14.6 | -1.1 | -1.7 | * | 0.3 | * | 0.4 | 0.1 |
| Yb | 0.7 | -0.4 | * | 0.1 | * | * | 0.2 | -10.0 | * | * | * | * |
| Zn | 1.2 | -0.3 | -0.6 | -0.8 | 9.4 | 106.9 | * | * | -0.8 | * | 0.0 | 1.0 |
| Zr | 0.8 | -3.3 | -1.7 | 2.9 | 31.8 | -1.1 | -0.9 | * | 0.0 | * | -0.5 | 2.9 |

| Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005) | | | | | | | | | | | | |
|---|-----------------------------|-------|-------|-------|-------|-------|-------|--------|-------|-------|-------|-------|
| | Quartz diorite KPT-1 | | | | | | | | | | | |
| Identifier | S22 | S23 | S23 | S24 | S25 | S25 | S26 | S27 | S28 | S28 | S29 | S30 |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Quality | 2 | 1 | 2 | 2 | 1 | 2 | 1 | 2 | 1 | 2 | 2 | 1 |
| SiO2 | * | * | * | 0.4 | 1.9 | * | 0.5 | -0.9 | 0.0 | * | -0.7 | 0.6 |
| TiO2 | * | * | -1.6 | -1.9 | -0.1 | * | -0.4 | 0.7 | 1.7 | * | -2.7 | -2.1 |
| Al2O3 | * | * | * | -1.3 | 0.4 | * | -0.4 | -0.9 | 1.7 | * | 0.3 | 0.4 |
| Fe2O3 | * | * | * | 1.4 | 0.6 | * | -1.1 | -1.9 | 1.7 | * | -0.7 | -0.6 |
| MnO | * | * | -1.8 | 0.8 | 0.6 | * | 2.1 | -0.6 | * | 0.0 | -1.8 | 0.0 |
| MgO | * | * | * | 0.9 | 1.4 | * | 3.1 | -0.5 | * | -0.7 | 7.9 | -0.9 |
| CaO | * | * | * | 0.4 | 0.0 | * | 2.6 | -1.4 | 0.3 | * | -0.2 | -0.7 |
| Na2O | * | * | * | -0.6 | 0.4 | * | -1.6 | -1.4 | * | * | 1.7 | -0.1 |
| K2O | * | * | * | -0.7 | -0.6 | * | 0.3 | -1.3 | * | * | 0.8 | -1.0 |
| P2O5 | * | * | * | 1.6 | 0.2 | * | -4.4 | -0.2 | * | -0.3 | 3.2 | -2.3 |
| Ba | * | -0.6 | * | -1.5 | 0.4 | * | -3.3 | 1.8 | * | -0.3 | -1.2 | * |
| Be | * | * | * | * | * | * | 6.8 | * | * | 1.2 | * | * |
| Bi | * | -1.8 | * | * | * | * | 0.3 | 10.9 | * | * | * | * |
| Ce | * | -1.1 | * | -0.6 | * | -0.8 | 1.3 | * | 2.8 | * | * | * |
| Cr | * | -2.3 | * | 1.6 | 3.4 | * | 2.9 | -1.8 | * | -0.6 | 1.0 | * |
| Cs | * | -0.8 | * | -1.2 | * | * | * | 4.9 | * | -2.5 | * | * |
| Dy | * | -0.2 | * | -0.2 | * | * | 2.0 | * | 0.4 | * | * | * |
| Er | * | -0.1 | * | -0.5 | * | * | 0.3 | * | 0.7 | * | * | * |
| Eu | * | -0.4 | * | 0.2 | * | * | -0.2 | * | 0.8 | * | * | * |
| Ga | * | 0.8 | * | * | * | * | * | 0.4 | -0.5 | * | -1.0 | * |
| Gd | * | 0.0 | * | -0.5 | * | * | 4.1 | * | * | 0.1 | * | * |
| Hf | * | -2.5 | * | -0.1 | * | * | * | 0.0 | * | 0.2 | * | * |
| Ho | * | -0.6 | * | 0.3 | * | * | 5.5 | * | -0.2 | * | * | * |
| La | * | -0.7 | * | -0.2 | * | -0.7 | 1.1 | 3.1 | 1.9 | * | * | * |
| Li | * | * | * | * | * | * | -1.6 | * | -0.7 | * | * | * |
| Lu | * | -0.3 | * | 0.0 | * | * | 3.6 | * | 0.0 | * | * | * |
| Mo | * | -11.2 | * | -2.4 | * | * | * | 0.4 | * | -0.9 | * | * |
| Nb | * | -1.6 | * | -1.2 | -0.4 | * | 1.0 | 0.9 | * | -1.5 | 0.9 | * |
| Nd | * | -0.5 | * | -0.3 | * | * | 1.4 | * | 1.0 | * | * | * |
| Pb | -3.3 | -1.2 | * | 6.7 | 0.6 | * | 0.6 | 1132.6 | * | -2.6 | -2.0 | * |
| Pr | * | -0.5 | * | -0.2 | * | * | 0.8 | * | 1.1 | * | * | * |
| Rb | * | -1.3 | * | -0.9 | -0.1 | * | -1.3 | 0.3 | -2.4 | * | -1.3 | * |
| Sb | * | 0.0 | * | 0.0 | * | * | -4.6 | -3.5 | 4.4 | * | * | * |
| Sc | * | 0.1 | * | -0.4 | * | * | * | -1.5 | 2.5 | * | * | * |
| Se | * | * | * | * | * | * | * | * | * | * | * | * |
| Sm | * | -1.9 | * | 0.2 | * | * | -0.7 | * | -0.1 | * | * | * |
| Sn | * | -0.1 | * | -0.8 | * | * | -10.3 | -1.1 | * | -0.9 | * | * |
| Sr | * | -3.9 | * | -1.2 | 0.1 | * | -0.8 | 0.7 | * | 0.9 | -1.1 | * |
| Ta | * | 0.2 | * | 0.4 | * | * | * | 0.1 | * | * | * | * |
| Tb | * | -0.5 | * | 0.2 | * | * | * | * | 1.1 | * | * | * |
| Th | * | -1.1 | * | -0.1 | * | 3.2 | * | 1.6 | 0.4 | * | 1.1 | * |
| Tl | * | -0.7 | * | * | * | * | * | * | * | 0.6 | * | * |
| Tm | * | -0.5 | * | 0.7 | * | * | -0.2 | * | 0.6 | * | * | * |
| U | * | -1.2 | * | 0.5 | * | -2.9 | * | -2.2 | 1.7 | * | * | * |
| V | * | -1.2 | * | 0.3 | 1.2 | * | -1.4 | 0.8 | * | 0.3 | 0.3 | * |
| Y | * | -1.4 | * | 0.7 | 1.5 | * | 1.7 | 0.9 | 2.2 | * | -1.0 | * |
| Yb | * | 0.1 | * | -0.2 | * | * | 5.1 | * | 0.6 | * | * | * |
| Zn | * | 5.9 | * | 1.9 | -0.1 | * | 2.9 | 4.4 | * | 1.5 | -1.3 | * |
| Zr | * | -4.8 | * | 0.7 | -0.3 | * | -1.2 | 0.6 | 6.2 | * | -0.9 | * |

| Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005) | | | | | | | | | | | | |
|---|-----------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|
| | Quartz diorite KPT-1 | | | | | | | | | | | |
| Identifier | S31 | S32 | S33 | S34 | S35 | S36 | S37 | S38 | S39 | S39 | S40 | S41 |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Quality | 1 | 2 | 1 | 1 | 1 | 2 | 2 | 2 | 1 | 2 | 1 | 2 |
| SiO2 | -5.2 | -0.4 | -0.1 | 0.6 | 1.1 | -1.8 | 0.2 | -0.8 | * | 0.4 | -1.2 | 0.6 |
| TiO2 | -1.4 | 0.2 | -1.3 | -0.4 | 2.9 | 0.1 | 0.1 | -1.3 | * | 0.3 | -2.1 | 0.7 |
| Al2O3 | -11.6 | 0.1 | 0.4 | 1.0 | -5.2 | 4.8 | 0.4 | -0.7 | * | 0.1 | -1.7 | 0.1 |
| Fe2O3 | -1.1 | 0.3 | 0.2 | 0.1 | 5.6 | -23.6 | 0.3 | -1.7 | * | 0.7 | -1.9 | 1.0 |
| MnO | -1.5 | -1.0 | 0.9 | -0.7 | 2.6 | -0.5 | 0.8 | -0.6 | * | 0.8 | -1.0 | -0.4 |
| MgO | -0.2 | 0.6 | 0.6 | 1.1 | -3.1 | 58.1 | 0.8 | -1.9 | * | 1.1 | -2.1 | 0.0 |
| CaO | -1.9 | -0.1 | -0.6 | 1.0 | 0.4 | 0.2 | -0.2 | -0.4 | * | 0.9 | -2.5 | -0.3 |
| Na2O | -17.2 | -0.4 | 1.0 | 0.6 | 8.5 | 0.3 | 0.3 | 1.9 | * | 0.3 | -2.3 | 1.6 |
| K2O | -2.4 | 0.0 | 0.2 | 0.3 | 3.9 | 1.1 | 0.7 | -0.2 | * | 0.0 | -2.6 | 0.0 |
| P2O5 | -1.3 | 0.6 | -0.4 | 3.2 | 0.9 | -0.7 | -0.7 | 0.6 | * | 1.6 | 5.5 | 0.9 |
| Ba | 0.6 | -0.3 | -0.4 | 2.3 | -0.2 | * | * | * | * | 0.3 | -2.4 | -0.4 |
| Be | * | * | -0.8 | -1.5 | -2.9 | * | * | * | * | -1.0 | * | * |
| Bi | 8.6 | * | * | -0.9 | -3.4 | * | * | * | * | 1.3 | * | -0.2 |
| Ce | 0.0 | 3.6 | -1.4 | -0.3 | 3.2 | * | * | * | * | 0.3 | * | -0.3 |
| Cr | -3.8 | 1.6 | 1.7 | 2.4 | -1.2 | -9.7 | * | * | * | 0.2 | -0.9 | 0.5 |
| Cs | 2.0 | 1.6 | 2.3 | 0.1 | 1.0 | * | * | * | * | -0.6 | * | 0.1 |
| Dy | * | 2.3 | 0.6 | 0.9 | 0.4 | * | * | * | * | 0.0 | * | -0.2 |
| Er | * | 3.4 | 0.9 | 0.4 | 0.0 | * | * | * | * | -0.2 | * | -0.1 |
| Eu | * | 0.7 | -0.2 | 0.3 | -0.2 | * | * | * | * | 0.3 | * | 0.0 |
| Ga | -1.9 | * | 1.0 | -0.1 | 1.1 | * | * | * | * | 0.7 | -4.5 | 0.4 |
| Gd | * | 3.1 | 0.2 | 0.8 | 0.6 | * | * | * | * | 0.1 | * | 0.1 |
| Hf | * | -0.8 | 1.8 | -0.1 | -0.3 | * | * | * | * | 0.0 | * | 0.1 |
| Ho | * | 1.8 | 0.4 | 0.2 | 0.3 | * | * | * | * | -0.3 | * | -0.5 |
| La | -2.5 | 1.9 | -1.3 | 0.5 | -2.1 | * | * | * | * | 0.4 | * | -0.1 |
| Li | * | * | * | 0.5 | -2.5 | * | * | * | * | * | * | * |
| Lu | * | 3.3 | 1.3 | 0.4 | 0.2 | * | * | * | * | 0.2 | * | 0.1 |
| Mo | * | -2.3 | 0.6 | 0.3 | -2.3 | * | * | * | * | -0.1 | * | 6.1 |
| Nb | -0.2 | 0.5 | -1.0 | 0.7 | 0.3 | -0.5 | * | * | * | -1.0 | 1.0 | -0.3 |
| Nd | * | 2.7 | 0.3 | 1.0 | 0.1 | * | * | * | * | 0.0 | * | 0.0 |
| Pb | -0.8 | -0.8 | 0.8 | 0.5 | 3.3 | * | * | * | * | 0.7 | -2.7 | -0.5 |
| Pr | * | 2.2 | -0.6 | 0.4 | -0.2 | * | * | * | * | 0.3 | * | -0.3 |
| Rb | -2.2 | 4.1 | -0.4 | -0.1 | 0.3 | 0.1 | * | * | * | -0.2 | -2.1 | 0.0 |
| Sb | 6.2 | * | 0.0 | 1.1 | 2.3 | * | * | * | * | 0.3 | * | -0.8 |
| Sc | * | * | 0.1 | -1.7 | -4.0 | * | * | * | * | * | -1.5 | 0.2 |
| Se | -11.7 | * | * | * | * | * | * | * | * | * | * | * |
| Sm | 5.8 | 2.6 | 0.4 | 0.7 | -0.2 | * | * | * | * | 0.3 | * | -0.6 |
| Sn | 2.4 | 4.3 | 1.0 | -0.5 | 2.0 | * | * | * | * | 0.1 | * | 0.6 |
| Sr | -2.8 | 2.5 | 0.4 | 1.0 | 0.8 | -0.5 | * | * | * | -0.4 | -3.1 | 0.6 |
| Ta | * | 10.9 | -2.2 | -0.7 | 21.2 | * | * | * | * | 0.9 | * | 0.0 |
| Tb | * | 3.0 | -0.8 | 0.6 | -0.3 | * | * | * | * | -0.1 | * | 0.6 |
| Th | 1.2 | -2.6 | -2.3 | -0.2 | -0.3 | -1.5 | * | * | * | 0.1 | 1.7 | 0.2 |
| Tl | 20.2 | * | * | -0.7 | 0.8 | * | * | * | * | * | * | -0.3 |
| Tm | * | 0.4 | * | 0.5 | 0.3 | * | * | * | * | -0.1 | * | -0.2 |
| U | 10.4 | 2.3 | 0.0 | -0.6 | 2.8 | 4.8 | * | * | * | 0.4 | * | -0.6 |
| V | -0.7 | -0.7 | 1.7 | 0.9 | 0.9 | * | * | * | * | -0.7 | -2.6 | -0.5 |
| Y | -0.7 | 9.5 | -3.5 | -0.3 | -1.1 | 0.1 | * | * | * | 0.0 | -1.4 | 0.0 |
| Yb | 90.2 | 3.0 | 0.6 | 0.5 | 0.3 | * | * | * | * | 0.2 | * | -0.9 |
| Zn | -1.0 | 8.4 | 0.5 | 0.4 | -1.1 | 0.0 | * | * | * | 0.9 | -2.4 | 1.7 |
| Zr | -0.8 | -3.1 | -0.2 | 0.9 | 1.0 | -0.7 | * | * | * | 0.8 | -1.7 | 1.0 |

| Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005) | | | | | | | | | | | | |
|---|-----------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|
| | Quartz diorite KPT-1 | | | | | | | | | | | |
| Identifier | S42 | S43 | S44 | S44 | S45 | S46 | S47 | S48 | S49 | S50 | S51 | S52 |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Quality | 1 | 2 | 1 | 2 | 1 | 2 | 2 | 1 | 2 | 2 | 2 | 2 |
| SiO2 | * | 0.3 | * | * | -0.5 | 0.4 | -0.8 | -2.7 | -0.5 | 0.6 | -0.4 | 0.5 |
| TiO2 | 2.3 | 0.9 | -1.5 | * | -0.1 | 0.9 | 0.1 | 2.8 | 0.1 | -0.2 | 1.2 | 0.2 |
| Al2O3 | * | -0.3 | -1.5 | * | -0.2 | 1.0 | -0.7 | -4.2 | -0.3 | 0.8 | -0.5 | 0.7 |
| Fe2O3 | * | 0.7 | 1.7 | * | 0.5 | 0.5 | 0.1 | -4.6 | -0.4 | -0.1 | 0.4 | 0.1 |
| MnO | 2.4 | -1.8 | -1.0 | * | 0.3 | 0.5 | -1.8 | -1.0 | -0.5 | -0.5 | 0.7 | 0.4 |
| MgO | * | -1.4 | -4.4 | * | 0.3 | 1.1 | 0.9 | -1.7 | -1.2 | 0.5 | 2.8 | -1.3 |
| CaO | * | -0.9 | -8.6 | * | -0.2 | -0.4 | 2.0 | -0.1 | -0.3 | 0.0 | 2.3 | 0.1 |
| Na2O | -0.5 | -0.5 | 1.5 | * | 0.4 | -0.2 | -2.3 | 5.7 | -0.7 | 0.6 | -0.3 | 0.2 |
| K2O | * | -1.0 | 4.6 | * | 0.0 | 0.0 | 0.5 | -1.6 | -0.3 | 0.0 | -0.2 | 0.0 |
| P2O5 | * | -1.8 | * | * | -0.6 | 0.5 | -4.1 | -1.4 | -0.7 | -0.7 | -0.9 | 0.7 |
| Ba | -2.9 | -0.1 | -1.0 | * | -0.5 | 0.0 | * | 0.2 | -0.2 | -1.0 | 1.5 | * |
| Be | * | 0.8 | * | * | * | -0.6 | * | * | * | * | * | * |
| Bi | * | * | * | * | * | -0.2 | * | -12.4 | * | * | * | * |
| Ce | 5.5 | -1.2 | 1.9 | * | -1.6 | 0.2 | * | 11.2 | 0.0 | -0.3 | 0.8 | * |
| Cr | 0.0 | 0.1 | 1.7 | * | -0.2 | 1.1 | -1.1 | 11.9 | * | -0.6 | -1.1 | * |
| Cs | -1.9 | * | -0.8 | * | -0.3 | 0.0 | * | -12.1 | 0.1 | -0.2 | -0.7 | * |
| Dy | -0.5 | -3.8 | 0.1 | * | 1.7 | 0.6 | * | -8.6 | -0.1 | 0.1 | -0.7 | * |
| Er | * | -3.8 | * | * | 0.3 | 0.0 | * | -3.8 | -0.1 | 0.2 | -0.7 | * |
| Eu | 1.0 | -2.6 | 1.7 | * | 0.7 | 0.0 | * | -2.5 | -0.2 | 1.3 | -0.3 | * |
| Ga | * | 0.9 | * | 0.4 | -0.7 | 0.4 | * | -2.4 | * | * | 5.6 | * |
| Gd | * | -3.1 | * | * | 0.7 | 0.1 | * | 4.8 | -0.2 | 0.0 | -0.4 | * |
| Hf | -0.2 | 2.1 | 1.7 | * | 0.7 | 0.0 | * | 23.4 | 0.4 | * | -1.8 | * |
| Ho | 0.6 | -3.6 | * | * | 0.8 | -0.2 | * | 0.6 | -0.1 | 0.4 | 0.2 | * |
| La | -0.5 | 0.4 | 1.0 | * | 0.1 | 0.2 | * | 4.6 | -0.2 | -0.3 | 1.6 | * |
| Li | * | 0.0 | * | * | * | 0.0 | * | * | * | 2.4 | -1.3 | * |
| Lu | -0.5 | -3.7 | 1.0 | * | 0.1 | -0.1 | * | * | -0.1 | 0.0 | -0.3 | * |
| Mo | * | * | * | * | * | -0.9 | * | -5.7 | * | * | * | * |
| Nb | * | 0.3 | * | * | -0.2 | 0.0 | * | -1.0 | 0.1 | * | 4.4 | * |
| Nd | -1.0 | -3.2 | 6.0 | * | -1.3 | 0.1 | * | 9.3 | 0.3 | 0.1 | 1.0 | * |
| Pb | * | -0.6 | * | * | 0.1 | -0.2 | * | -1.8 | 0.3 | -0.7 | -3.3 | * |
| Pr | * | -1.8 | * | * | -1.5 | 0.1 | * | 9.3 | 0.1 | 0.1 | 0.8 | * |
| Rb | 0.7 | -0.5 | 1.7 | * | -0.1 | 0.6 | * | -0.6 | 1.0 | 0.8 | -1.3 | * |
| Sb | 0.2 | -1.8 | -0.5 | * | * | 1.0 | * | -12.4 | * | 0.7 | * | * |
| Sc | -0.5 | -0.3 | 0.6 | * | 0.7 | 0.1 | * | 9.9 | 1.1 | 1.0 | 0.1 | * |
| Se | 2.2 | * | * | 1.4 | * | 2.7 | * | * | * | * | * | * |
| Sm | -0.6 | * | 0.7 | * | 0.8 | -0.2 | * | 16.5 | -0.1 | 0.3 | 1.7 | * |
| Sn | * | -1.1 | * | * | * | 0.4 | * | -13.4 | * | * | 5.9 | * |
| Sr | -2.9 | -0.2 | * | 3.3 | -0.8 | 0.2 | * | -0.2 | 0.5 | 3.5 | 0.6 | * |
| Ta | -1.7 | * | * | -0.9 | 0.6 | 1.0 | * | -11.6 | 0.0 | * | 2.1 | * |
| Tb | -0.6 | -3.2 | 0.5 | * | 1.0 | -0.3 | * | 36.5 | -0.1 | -0.2 | 0.3 | * |
| Th | -0.2 | * | -0.6 | * | 0.2 | -0.4 | * | -2.9 | -0.6 | 5.1 | -0.3 | * |
| Tl | * | * | * | * | * | 0.1 | * | * | * | * | * | * |
| Tm | * | * | * | * | 0.1 | 0.0 | * | * | 0.0 | -0.1 | -0.2 | * |
| U | -1.2 | * | * | -0.2 | -0.6 | 0.0 | * | 1.9 | -0.3 | 0.2 | -0.2 | * |
| V | 3.6 | 0.1 | 1.5 | * | -0.2 | 0.5 | 14.2 | -0.3 | * | -1.6 | 0.2 | * |
| Y | * | 0.1 | * | * | 1.2 | 0.1 | * | 0.1 | -0.5 | -0.3 | 1.1 | * |
| Yb | -0.5 | -4.7 | 0.9 | * | -0.1 | 0.0 | * | -3.7 | 0.0 | 0.0 | -1.3 | * |
| Zn | -8.0 | -0.1 | * | -5.4 | -1.0 | 0.2 | -3.8 | 1.0 | * | 0.6 | -2.9 | * |
| Zr | -19.5 | -1.0 | * | 4.4 | 2.1 | 0.6 | * | -0.2 | 1.9 | 2.0 | -2.6 | * |

| Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005) | | | | | | | | | | | | |
|---|-----------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|
| | Quartz diorite KPT-1 | | | | | | | | | | | |
| Identifier | S53 | S54 | S55 | S55 | S56 | S57 | S58 | S59 | S60 | S61 | S62 | S63 |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Quality | 1 | 2 | 1 | 2 | 2 | 2 | 2 | 1 | 1 | 1 | 1 | 1 |
| SiO2 | * | 2.0 | 0.0 | * | * | 0.2 | 0.3 | 0.4 | 0.1 | 0.0 | * | -7.8 |
| TiO2 | 3.9 | -1.0 | 0.5 | * | 1.4 | 0.8 | 0.3 | 0.7 | -0.1 | 2.3 | -0.4 | -2.5 |
| Al2O3 | 2.5 | -3.4 | -0.2 | * | 1.7 | 0.7 | 0.1 | 0.6 | 0.1 | 3.8 | * | -9.3 |
| Fe2O3 | -0.2 | -3.1 | 0.4 | * | -0.4 | 0.3 | 0.2 | 0.8 | -0.2 | 0.7 | * | 3.5 |
| MnO | -1.0 | -4.4 | 1.6 | * | 2.1 | 0.7 | 0.8 | -1.0 | 0.6 | 4.2 | -3.6 | -0.7 |
| MgO | -0.1 | -5.5 | -1.4 | * | * | 0.4 | 0.0 | -0.5 | 0.6 | * | * | -4.8 |
| CaO | -2.8 | -4.2 | 0.1 | * | * | 0.9 | -1.1 | 1.4 | 0.0 | -0.4 | * | -6.4 |
| Na2O | 4.1 | 15.8 | -1.2 | * | 126.6 | -0.4 | -0.7 | -3.8 | -0.9 | -4.1 | 1.5 | * |
| K2O | 4.9 | 3.3 | -1.3 | * | 297.0 | -0.6 | 0.2 | 0.0 | -0.1 | 9.5 | 2.9 | -1.6 |
| P2O5 | -1.4 | -7.6 | 0.2 | * | * | 0.3 | 0.5 | 0.9 | 6.2 | 3.2 | 0.9 | * |
| Ba | 2.4 | * | * | 6.0 | * | 0.0 | 2.0 | 0.2 | 0.4 | 1.5 | 3.0 | * |
| Be | -0.2 | * | * | * | * | 0.8 | * | * | 0.2 | * | * | * |
| Bi | * | * | * | * | * | * | * | * | -1.3 | * | * | * |
| Ce | * | * | * | * | * | 0.1 | -2.6 | -1.8 | 0.0 | 2.6 | -1.1 | * |
| Cr | -0.4 | 0.9 | 2.3 | * | * | -0.1 | 0.8 | 1.2 | 4.7 | 2.4 | -2.7 | * |
| Cs | * | * | * | * | * | 0.3 | * | * | 0.4 | * | * | * |
| Dy | * | * | * | * | * | 0.3 | * | -1.4 | 2.4 | * | * | * |
| Er | * | * | * | * | * | 0.4 | * | -1.1 | -0.1 | * | * | * |
| Eu | * | * | * | * | * | 0.6 | * | -0.3 | 0.1 | * | * | * |
| Ga | 7.2 | * | 10.6 | * | * | 0.1 | -0.6 | 1.3 | 0.1 | -3.4 | * | * |
| Gd | * | * | * | * | * | 0.0 | * | -0.6 | 0.6 | * | * | * |
| Hf | * | * | * | * | * | 0.3 | 9.9 | * | -0.2 | * | * | * |
| Ho | * | * | * | * | * | 0.6 | * | -1.6 | 0.8 | * | * | * |
| La | 0.8 | * | * | * | * | 0.3 | 1.9 | -2.2 | 1.3 | -2.2 | * | * |
| Li | 1.2 | * | * | * | * | * | * | * | 4.8 | * | * | * |
| Lu | * | * | * | * | * | 0.0 | * | -1.6 | 0.5 | * | * | * |
| Mo | 2.2 | * | * | * | * | * | * | * | * | * | * | * |
| Nb | * | * | 2.1 | * | * | -0.3 | -1.5 | * | -2.8 | 5.1 | * | * |
| Nd | * | * | * | * | * | 0.3 | 1.0 | -1.8 | -0.4 | * | * | * |
| Pb | 0.6 | -1.1 | -8.6 | * | -5.5 | * | -0.2 | 6.0 | 0.0 | 0.0 | -3.9 | * |
| Pr | * | * | * | * | * | 0.2 | * | -0.8 | -1.1 | * | * | * |
| Rb | * | * | -0.4 | * | * | 0.7 | -0.3 | 1.5 | -0.1 | 2.9 | -5.1 | * |
| Sb | 1.8 | * | * | * | * | * | * | * | 1.3 | * | * | * |
| Sc | * | * | * | * | * | -0.2 | * | 1.9 | 0.6 | -0.7 | 0.9 | * |
| Se | 0.8 | * | * | * | * | * | * | * | -2.0 | * | * | * |
| Sm | * | * | * | * | * | 0.5 | * | -1.2 | 1.4 | * | * | * |
| Sn | -2.2 | * | * | * | * | * | -1.1 | * | 1.5 | * | * | * |
| Sr | 2.1 | * | 1.4 | * | * | 2.3 | -0.3 | -0.3 | 1.5 | 0.3 | -2.0 | * |
| Ta | * | * | * | * | * | 0.4 | * | * | 0.8 | * | * | * |
| Tb | * | * | * | * | * | 0.2 | * | -0.8 | 0.6 | * | * | * |
| Th | * | * | -6.2 | * | * | 0.0 | 0.8 | -2.9 | 0.2 | * | -9.9 | * |
| Tl | * | * | * | * | * | * | * | * | 0.1 | * | * | * |
| Tm | * | * | * | * | * | 0.3 | * | -1.0 | 0.9 | * | * | * |
| U | * | * | * | * | * | 0.3 | * | 0.9 | -0.3 | * | * | * |
| V | -1.0 | * | 6.9 | * | * | -1.0 | 0.3 | -2.3 | 1.2 | 3.3 | -0.6 | * |
| Y | * | * | 7.4 | * | * | 0.8 | -0.3 | -0.7 | 0.5 | 7.2 | -14.1 | * |
| Yb | * | * | * | * | * | 0.1 | * | -1.4 | 1.1 | * | * | * |
| Zn | 4.2 | -0.1 | -4.2 | * | -3.6 | 1.1 | -0.8 | -0.4 | 1.1 | -3.0 | -2.6 | * |
| Zr | * | -0.2 | -3.0 | * | * | 0.9 | 0.8 | 1.3 | -0.3 | -0.2 | -6.5 | * |

| Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005) | | | | | | | | | | | | |
|---|-----------------------------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|-------|
| | Quartz diorite KPT-1 | | | | | | | | | | | |
| Identifier | S64 | S65 | S66 | S67 | S68 | S68 | S69 | S70 | S71 | S72 | S73 | S74 |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 |
| Quality | 1 | 1 | 2 | 2 | 1 | 2 | 2 | 2 | 2 | 1 | 2 | 2 |
| SiO2 | * | * | -0.1 | -0.4 | -1.3 | * | 1.0 | 0.3 | -1.0 | * | * | -0.8 |
| TiO2 | * | * | 1.9 | -0.5 | 0.6 | * | -1.0 | -0.5 | 0.1 | * | -1.0 | -0.2 |
| Al2O3 | * | * | 0.5 | -0.1 | -0.9 | * | -0.5 | -0.3 | -0.8 | * | * | -1.1 |
| Fe2O3 | * | -0.1 | 2.0 | -0.6 | 0.0 | * | -0.1 | 0.9 | -0.7 | * | -0.3 | -0.1 |
| MnO | * | * | -0.5 | 0.7 | 1.3 | * | 0.8 | -0.5 | -0.5 | * | 0.8 | -1.8 |
| MgO | * | * | 0.8 | -0.3 | 0.8 | * | 0.0 | -0.5 | 0.0 | * | * | 0.7 |
| CaO | * | * | 0.8 | -0.3 | 0.9 | * | -0.6 | 0.1 | 0.8 | * | -0.5 | -0.4 |
| Na2O | * | * | -0.6 | 0.1 | -1.0 | * | 0.3 | 0.3 | -0.2 | * | * | -2.4 |
| K2O | * | * | 1.0 | -0.3 | 0.0 | * | -0.2 | 0.5 | -0.3 | * | 4.7 | -0.8 |
| P2O5 | * | * | -3.2 | -0.7 | 0.5 | * | -1.8 | -0.7 | -0.7 | * | * | 5.1 |
| Ba | -0.5 | -2.1 | 3.8 | 2.0 | 0.0 | * | -0.3 | 2.2 | -0.9 | 0.8 | * | 0.1 |
| Be | * | * | 1.4 | -0.4 | * | * | -0.1 | * | 0.8 | * | * | * |
| Bi | * | * | * | 8.9 | * | * | * | * | 0.8 | * | * | * |
| Ce | -1.2 | -0.5 | 0.0 | -0.3 | 0.0 | * | -0.3 | * | -0.7 | -4.8 | * | 1.9 |
| Cr | * | * | 1.7 | 0.2 | 0.3 | * | -0.2 | -0.6 | -1.5 | 1.5 | -3.7 | -2.3 |
| Cs | 0.0 | -1.5 | 0.3 | -0.1 | -0.2 | * | -0.2 | * | -0.4 | * | * | * |
| Dy | -0.8 | * | 0.0 | 0.1 | -0.2 | * | 0.1 | * | 0.1 | * | * | * |
| Er | -0.9 | * | 0.3 | 0.0 | -0.1 | * | 0.1 | * | 0.9 | * | * | * |
| Eu | -1.3 | 0.4 | 0.2 | 0.1 | -0.5 | * | -0.3 | * | -0.2 | * | * | * |
| Ga | * | * | -0.1 | 0.0 | -0.2 | * | 0.0 | * | -0.1 | 0.8 | -2.8 | * |
| Gd | -1.2 | * | 0.0 | -0.1 | -1.2 | * | -0.2 | * | 0.1 | * | * | * |
| Hf | * | 0.7 | -0.1 | -1.3 | -1.2 | * | -0.7 | * | -0.7 | * | * | * |
| Ho | -1.1 | * | -0.2 | 0.1 | 0.2 | * | -0.2 | * | -0.4 | * | * | * |
| La | -1.4 | 0.0 | 0.0 | -0.3 | -2.3 | * | -0.2 | * | 0.1 | 0.8 | * | 0.0 |
| Li | * | * | * | -0.6 | * | * | 0.7 | * | -1.6 | * | * | 1.5 |
| Lu | -0.5 | -1.6 | -0.3 | -0.1 | 0.0 | * | -0.2 | * | 0.3 | * | * | * |
| Mo | * | * | 2.2 | -0.1 | * | * | 1.0 | * | * | * | * | * |
| Nb | -1.0 | * | 1.8 | -1.2 | -1.8 | * | -0.2 | * | 0.5 | 1.0 | * | * |
| Nd | -0.7 | 2.8 | -0.1 | 0.2 | 0.2 | * | -0.1 | * | -0.1 | * | * | * |
| Pb | -1.4 | * | -0.6 | 0.3 | 0.3 | * | 0.0 | 0.6 | 1.0 | -2.7 | * | 1.2 |
| Pr | -1.4 | * | 0.1 | 0.0 | 0.3 | * | -0.1 | * | -0.1 | * | * | * |
| Rb | -0.9 | -2.3 | 0.1 | -0.3 | -1.4 | * | -0.1 | * | 0.5 | 0.6 | 0.5 | * |
| Sb | * | * | -0.5 | -0.2 | * | * | 0.3 | * | 1.2 | * | * | * |
| Sc | * | -0.1 | * | 0.0 | -0.9 | * | -0.1 | * | 0.8 | 0.1 | * | * |
| Se | * | * | 0.0 | -1.1 | * | * | -1.7 | * | * | * | * | * |
| Sm | -1.2 | 0.0 | 0.1 | -0.4 | 0.2 | * | 0.0 | * | 0.0 | * | * | * |
| Sn | * | * | -0.1 | -0.1 | * | * | 0.2 | * | 0.7 | * | * | * |
| Sr | -0.8 | * | 0.9 | -0.3 | -0.2 | * | -0.5 | * | 0.6 | 1.1 | 0.5 | -1.7 |
| Ta | -1.5 | -2.5 | -0.3 | * | -6.7 | * | -0.6 | * | * | * | * | * |
| Tb | -1.2 | 1.8 | 0.0 | 0.0 | -1.1 | * | -0.2 | * | 0.2 | * | * | * |
| Th | 0.5 | 0.1 | 5.0 | 0.1 | -0.9 | * | -0.5 | * | 0.7 | 1.7 | * | * |
| Tl | * | * | * | -3.4 | * | * | 0.3 | * | 0.4 | * | * | * |
| Tm | -0.7 | * | -0.1 | 0.1 | 0.3 | * | -0.1 | * | -0.2 | * | * | * |
| U | 0.0 | -0.6 | * | 0.1 | -0.8 | * | -0.4 | * | 0.0 | 9.6 | * | * |
| V | * | * | -1.8 | -0.1 | 0.7 | * | -0.4 | * | 0.3 | 1.0 | * | -2.0 |
| Y | 0.1 | * | -0.9 | 0.0 | 0.0 | * | -0.5 | * | 0.1 | 0.1 | -1.1 | -1.1 |
| Yb | -2.0 | 1.1 | -0.1 | -0.1 | -0.4 | * | 0.0 | * | 0.3 | * | * | * |
| Zn | * | -0.5 | 1.5 | 0.3 | -0.1 | * | -1.4 | 1.0 | 0.1 | 0.4 | 0.1 | 2.0 |
| Zr | * | * | 0.1 | 0.4 | 1.0 | * | -0.2 | * | 0.0 | -0.7 | -0.7 | -0.3 |

Table 3 GeoPT18 Z-scores for results submitted (Dec. 2005)

| Quartz diorite KPT-1 | | | | | | |
|-----------------------------|-------|-------|-------|-------|-------|--|
| Identifier | S75 | S76 | S77 | S78 | S79 | |
| Sample | KPT-1 | KPT-1 | KPT-1 | KPT-1 | KPT-1 | |
| Quality | 2 | 1 | 1 | 1 | 1 | |
| SiO2 | -0.1 | -0.6 | 0.7 | 0.45 | 0.11 | |
| TiO2 | 0.2 | -2.6 | 1.2 | 0.10 | 3.77 | |
| Al2O3 | 1.6 | 0.5 | 4.8 | 1.50 | -2.80 | |
| Fe2O3 | 0.9 | -1.6 | -2.0 | 2.16 | 1.86 | |
| MnO | 0.2 | -2.3 | 9.4 | 1.61 | -4.11 | |
| MgO | 1.2 | -0.1 | -8.3 | -8.31 | -7.59 | |
| CaO | 0.3 | -0.9 | 2.6 | 2.55 | -0.17 | |
| Na2O | 1.8 | -1.0 | -7.6 | 3.23 | 1.46 | |
| K2O | -1.1 | -2.9 | 1.6 | 3.59 | 2.94 | |
| P2O5 | 0.5 | 0.9 | 10.1 | 10.13 | 15.41 | |
| Ba | -5.4 | * | 3.0 | | -31.5 | |
| Be | * | * | * | | | |
| Bi | * | * | * | | | |
| Ce | -0.3 | * | -6.9 | | | |
| Cr | -4.0 | * | 2.2 | | -26.6 | |
| Cs | * | * | * | | | |
| Dy | 0.1 | * | -5.1 | | | |
| Er | -0.1 | * | 54.5 | | | |
| Eu | 0.2 | * | -6.7 | | | |
| Ga | -1.2 | * | * | | | |
| Gd | -0.2 | * | 35.2 | | | |
| Hf | * | * | * | | | |
| Ho | -0.2 | * | * | | | |
| La | -0.5 | * | -5.3 | | | |
| Li | * | * | -4.9 | | | |
| Lu | -0.1 | * | * | | | |
| Mo | * | * | * | | | |
| Nb | * | * | 137.3 | | -17.2 | |
| Nd | 0.3 | * | -3.8 | | | |
| Pb | -0.8 | * | 87.2 | | -24.2 | |
| Pr | -0.1 | * | * | | | |
| Rb | 0.5 | * | * | | | |
| Sb | * | * | * | | | |
| Sc | -0.9 | * | 12.4 | | | |
| Se | * | * | * | | | |
| Sm | -0.1 | * | -12.6 | | | |
| Sn | * | * | * | | | |
| Sr | -0.4 | * | -4.1 | | -28.9 | |
| Ta | * | * | 356.2 | | | |
| Tb | -0.3 | * | * | | | |
| Th | -1.8 | * | * | | | |
| Tl | * | * | * | | | |
| Tm | -0.2 | * | * | | | |
| U | * | * | * | | | |
| V | -3.7 | * | * | | -27.7 | |
| Y | -1.2 | * | -2.2 | | -20.4 | |
| Yb | -0.1 | * | 0.1 | | | |
| Zn | 0.4 | * | -5.6 | | -25.7 | |
| Zr | -0.3 | * | * | | -26.8 | |

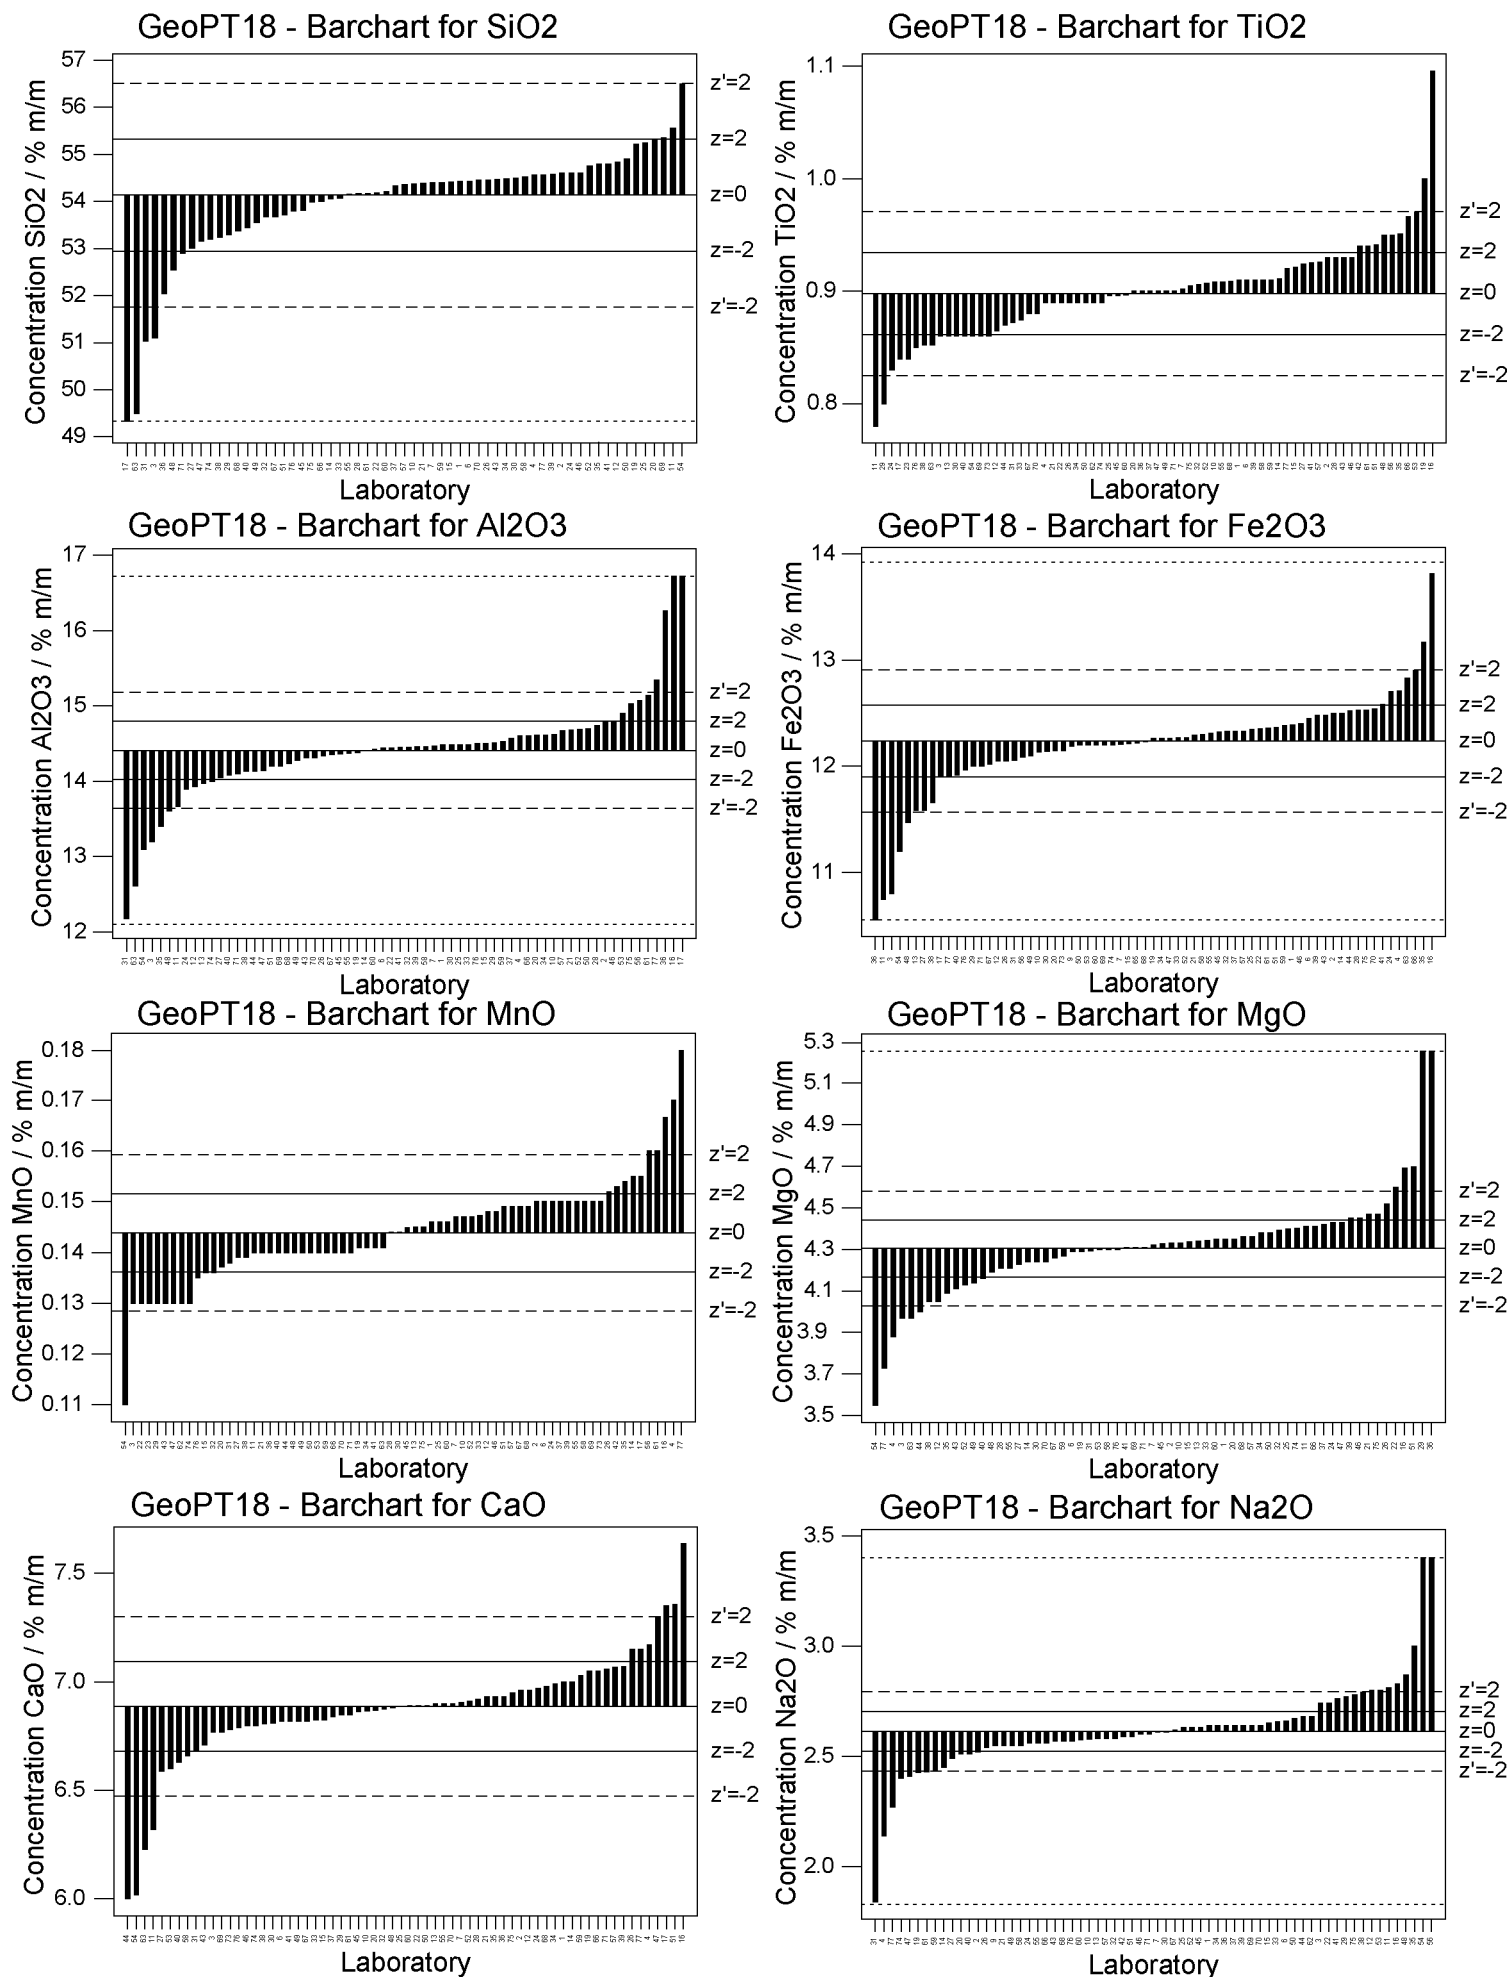


Figure 1: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

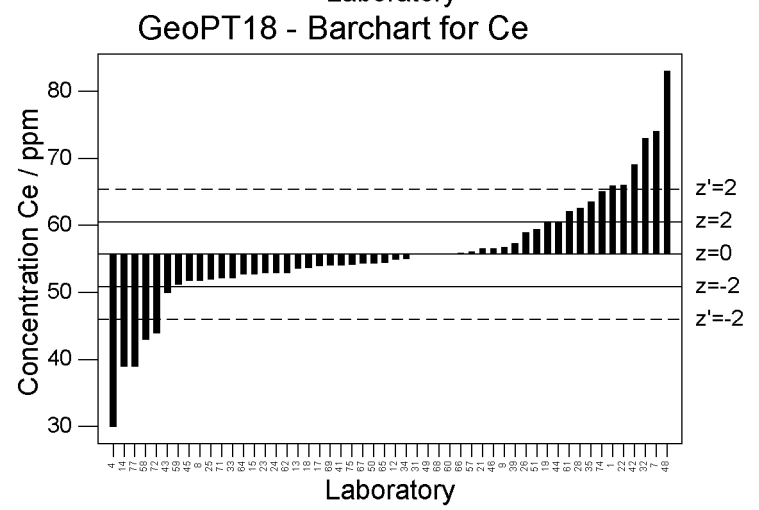
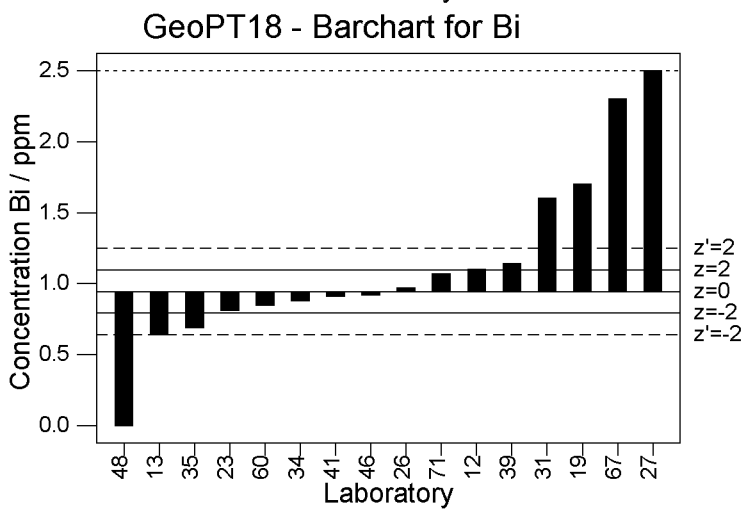
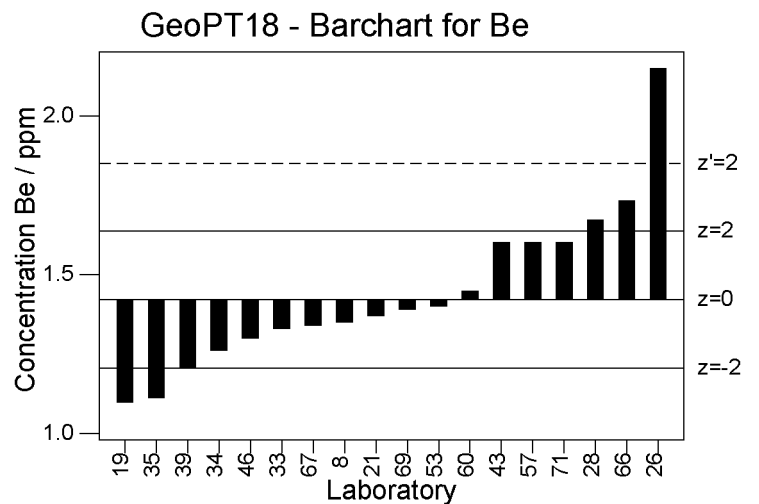
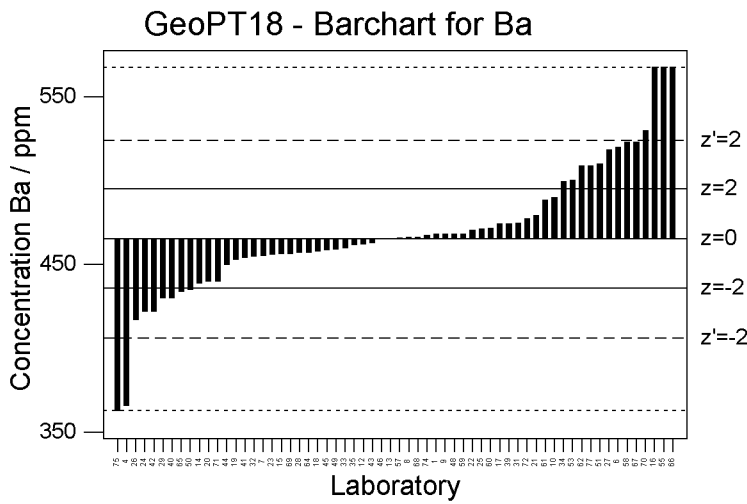
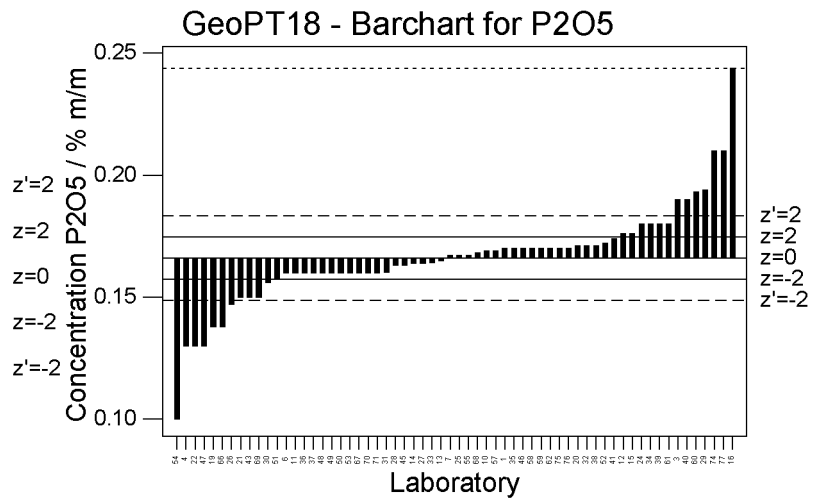
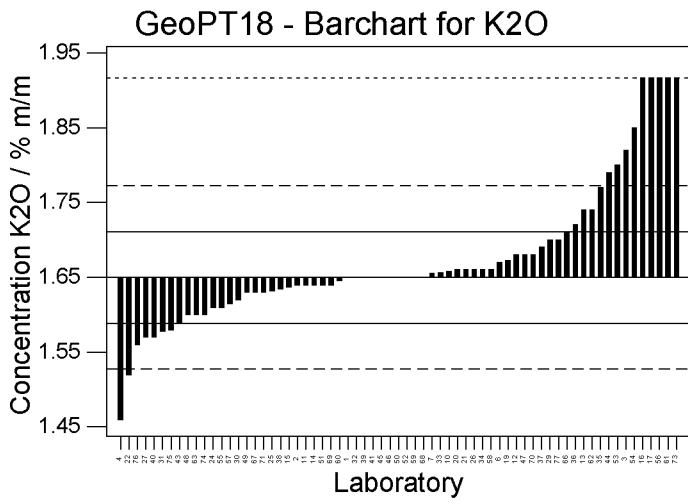


Figure 1: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

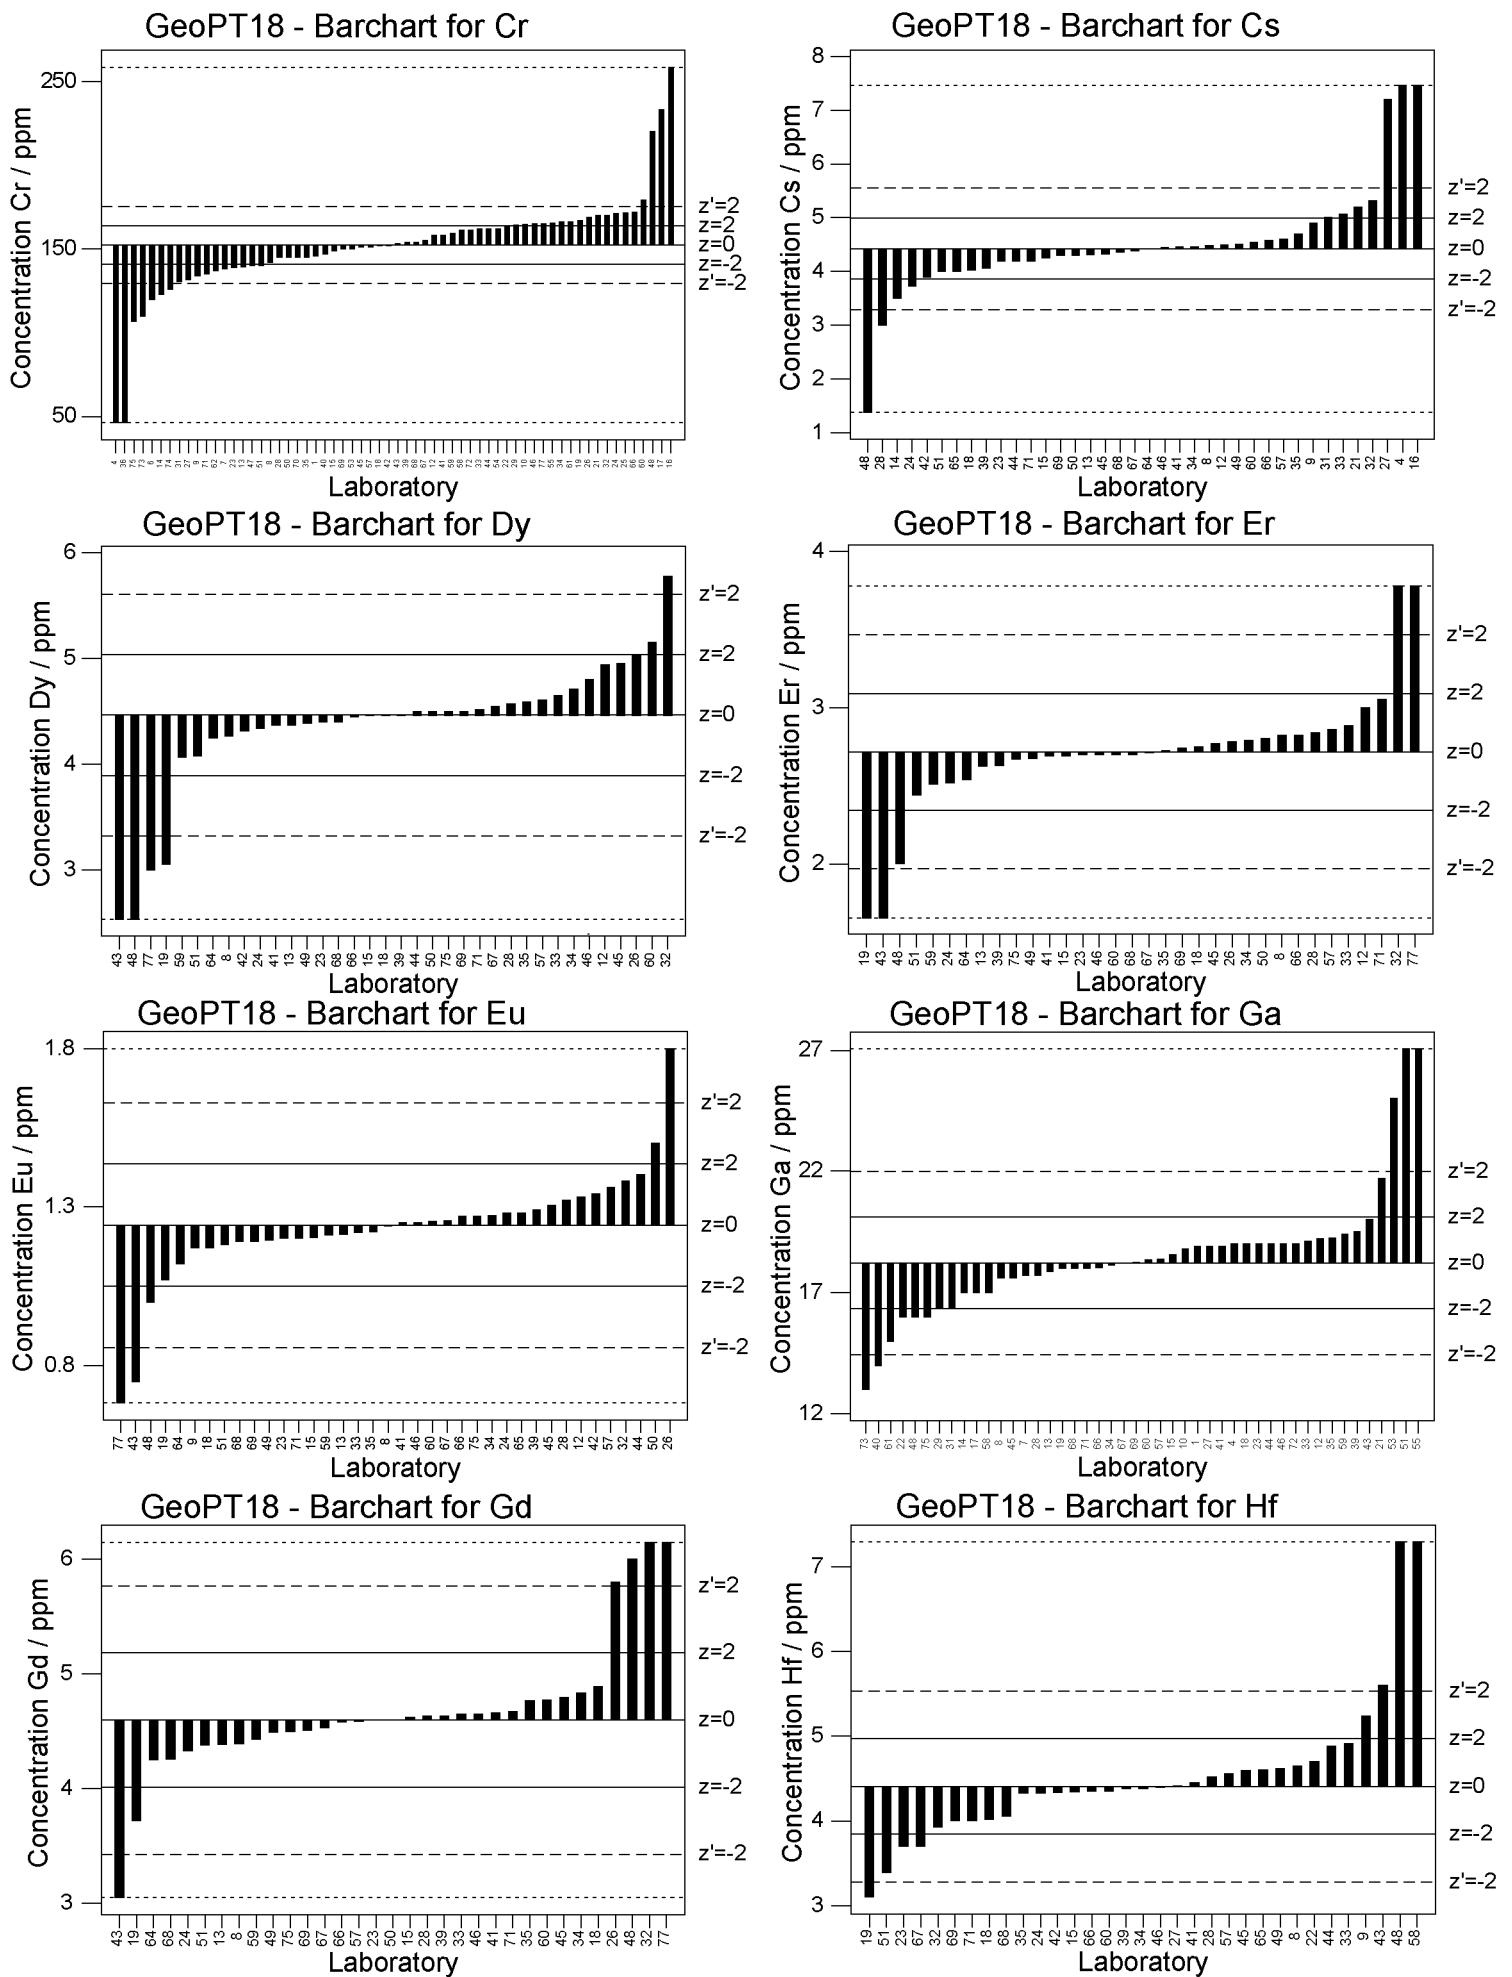


Figure 1: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

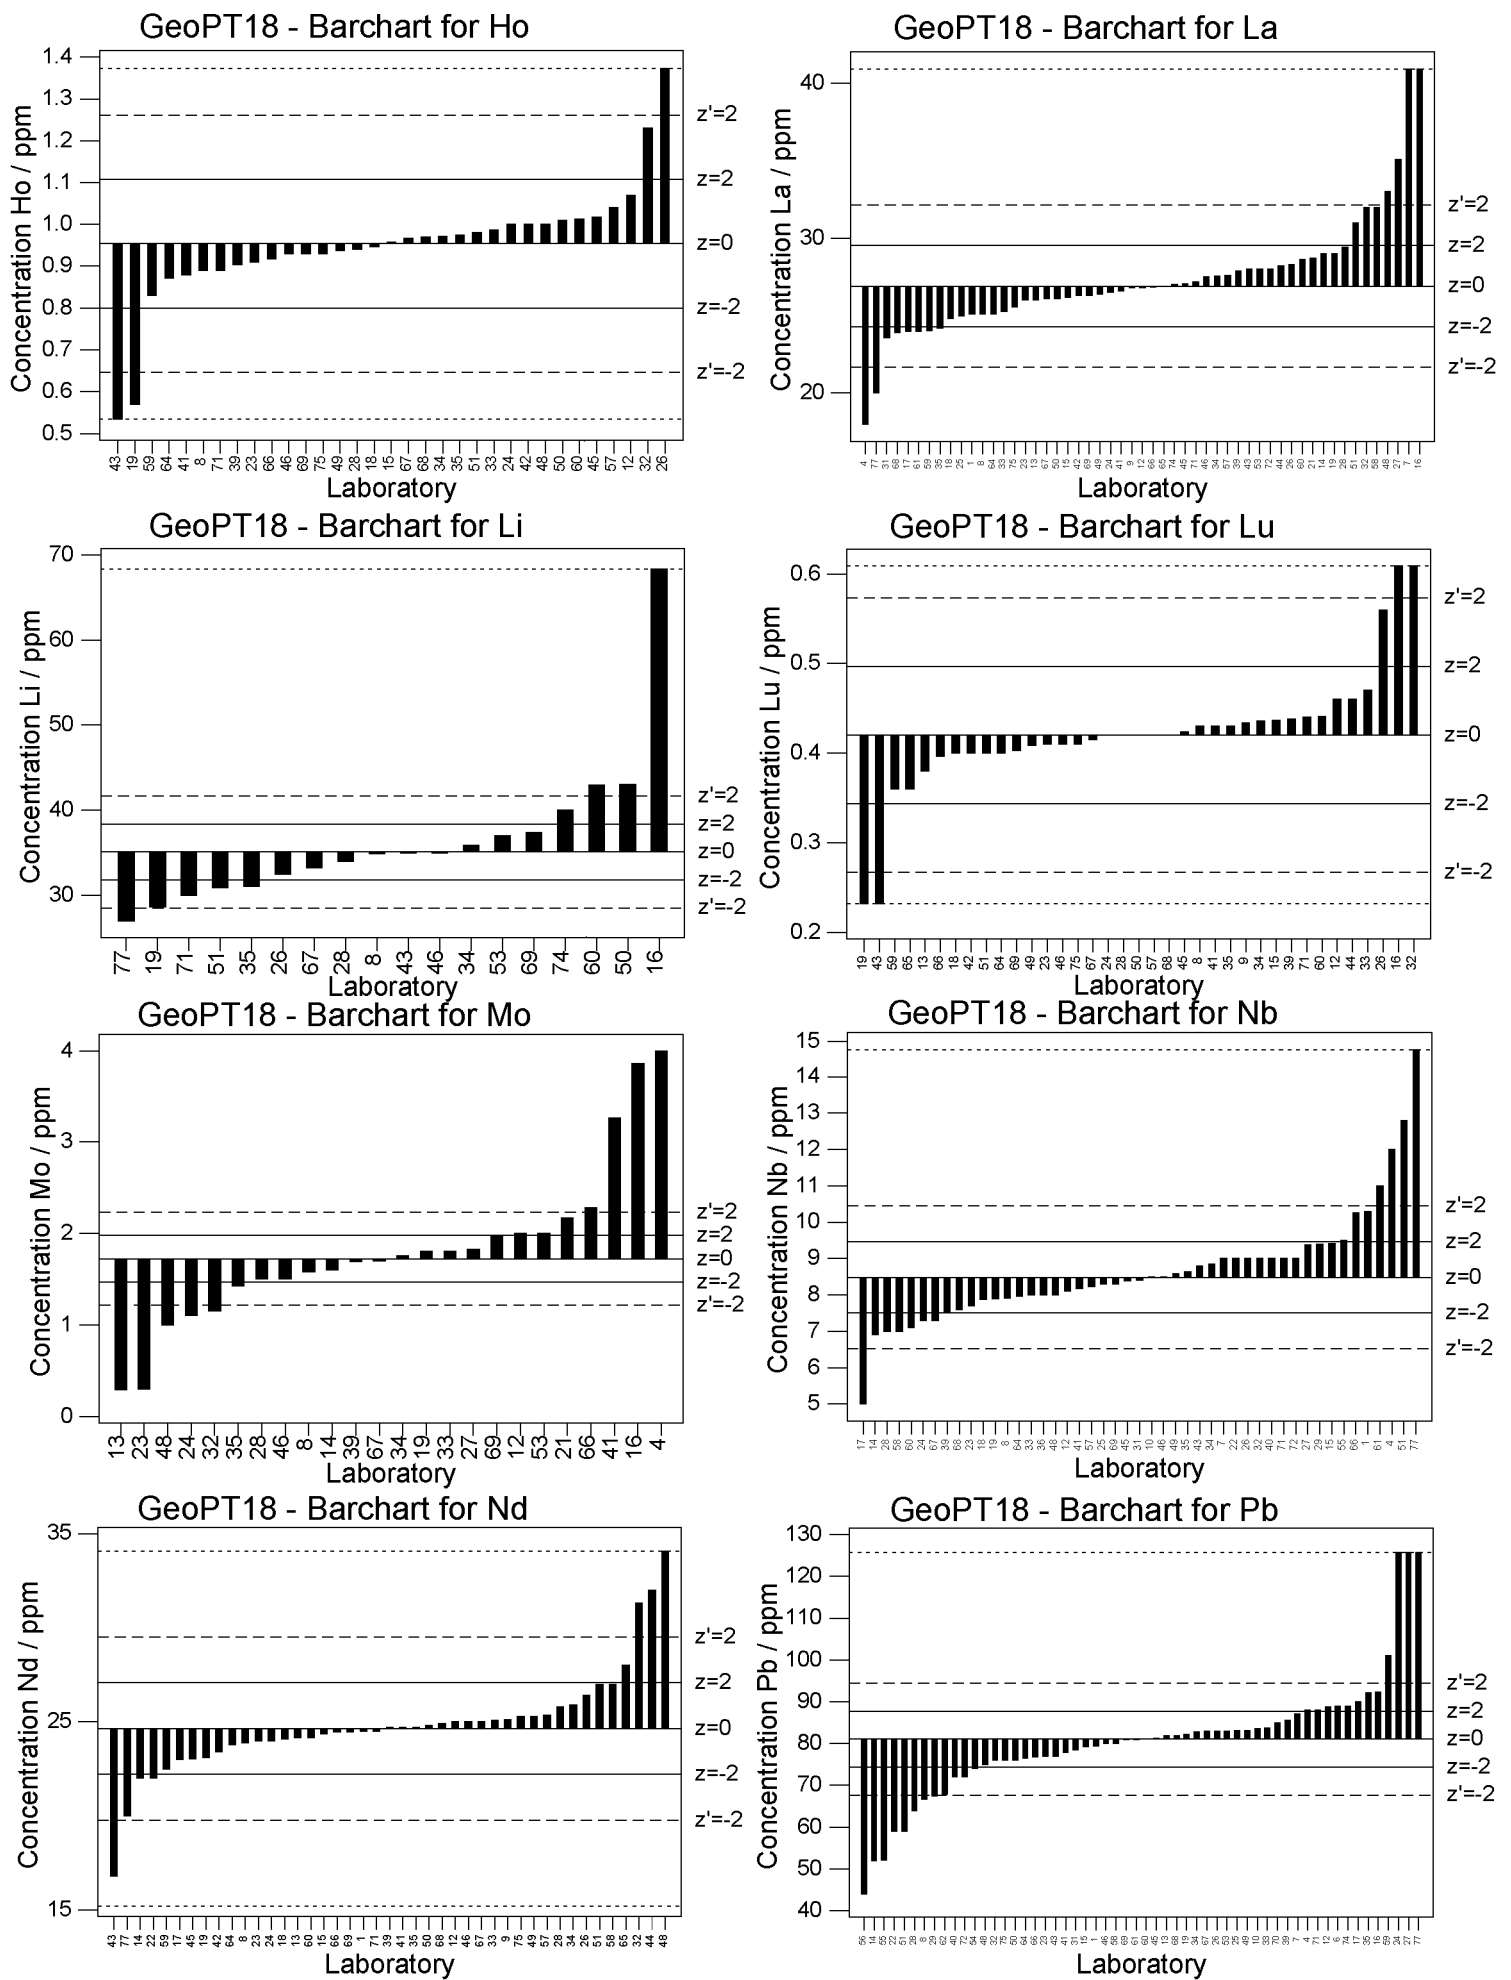


Figure 1: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

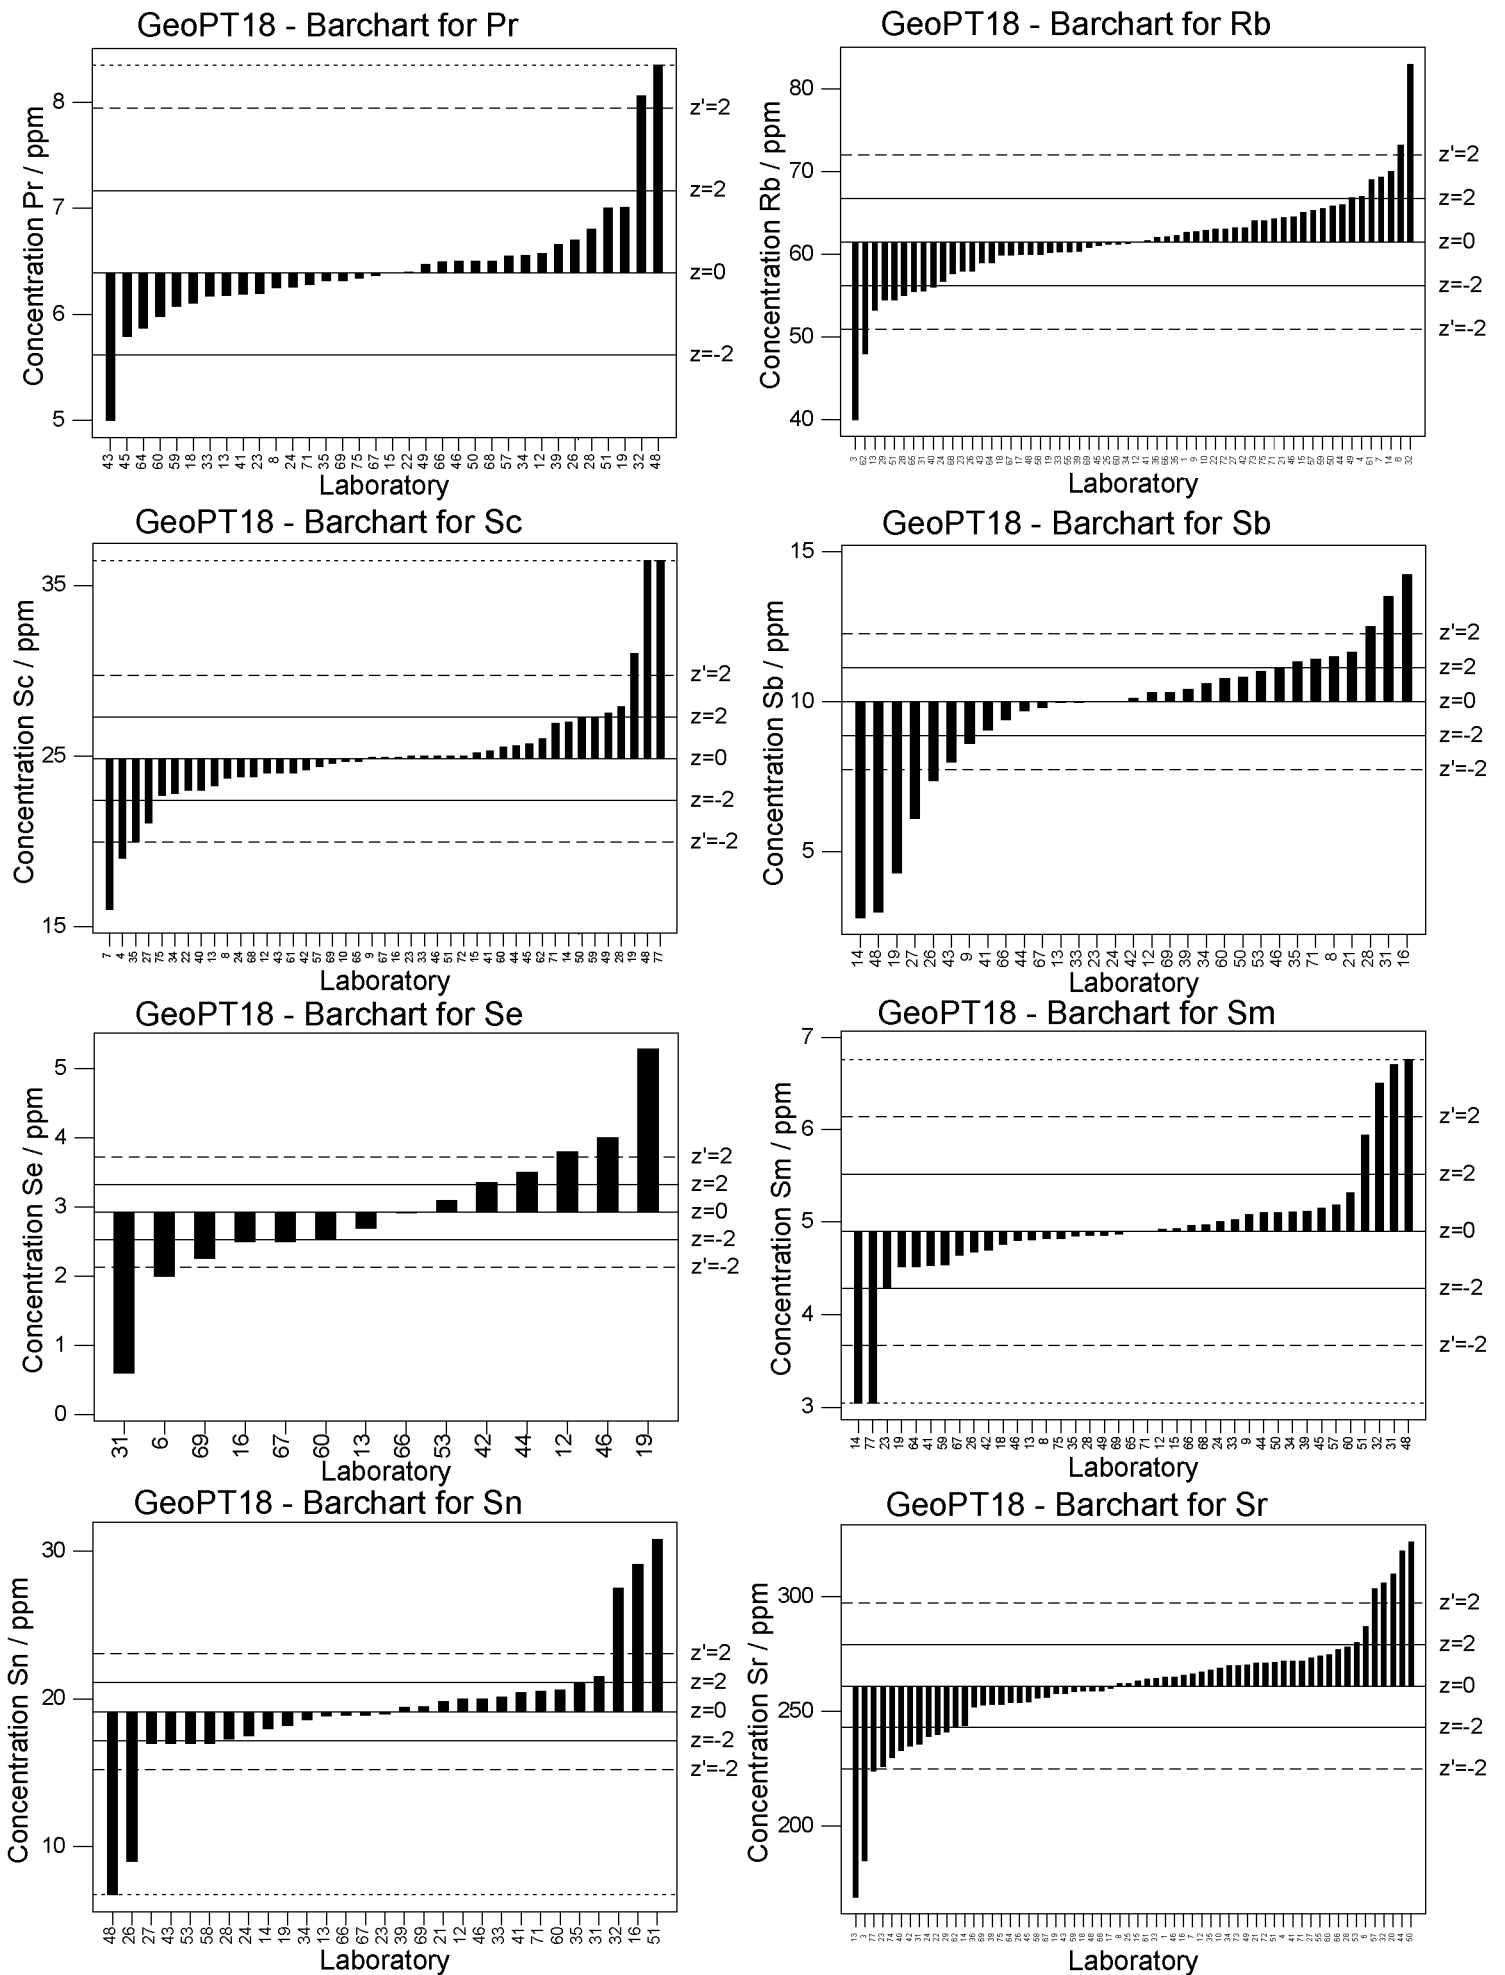


Figure 1: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

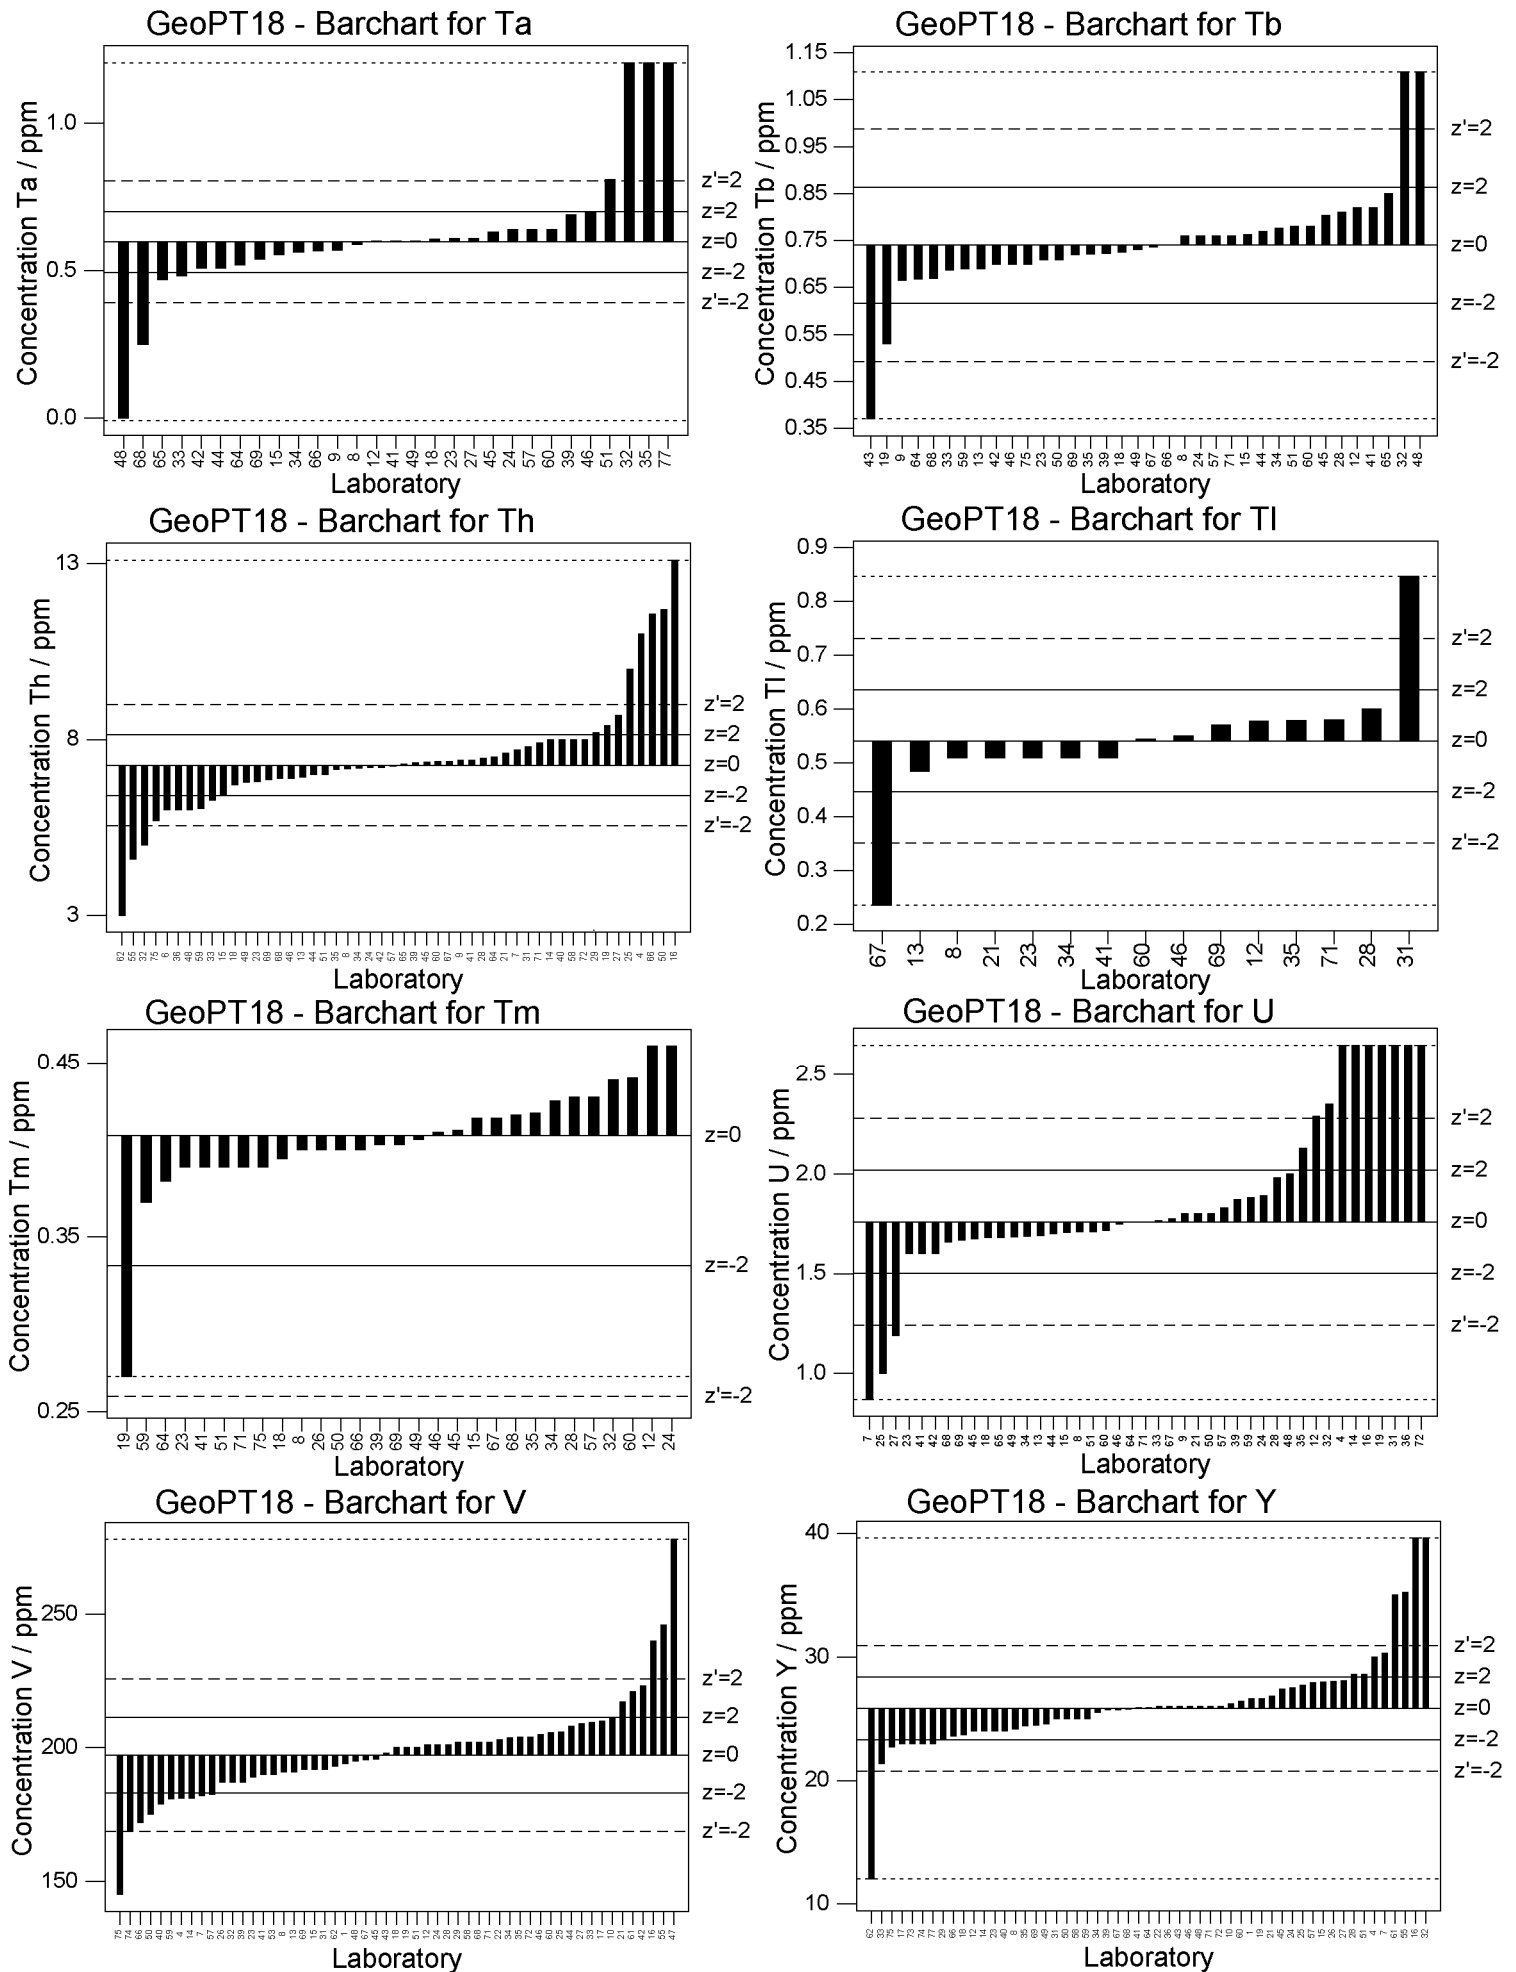


Figure 1: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

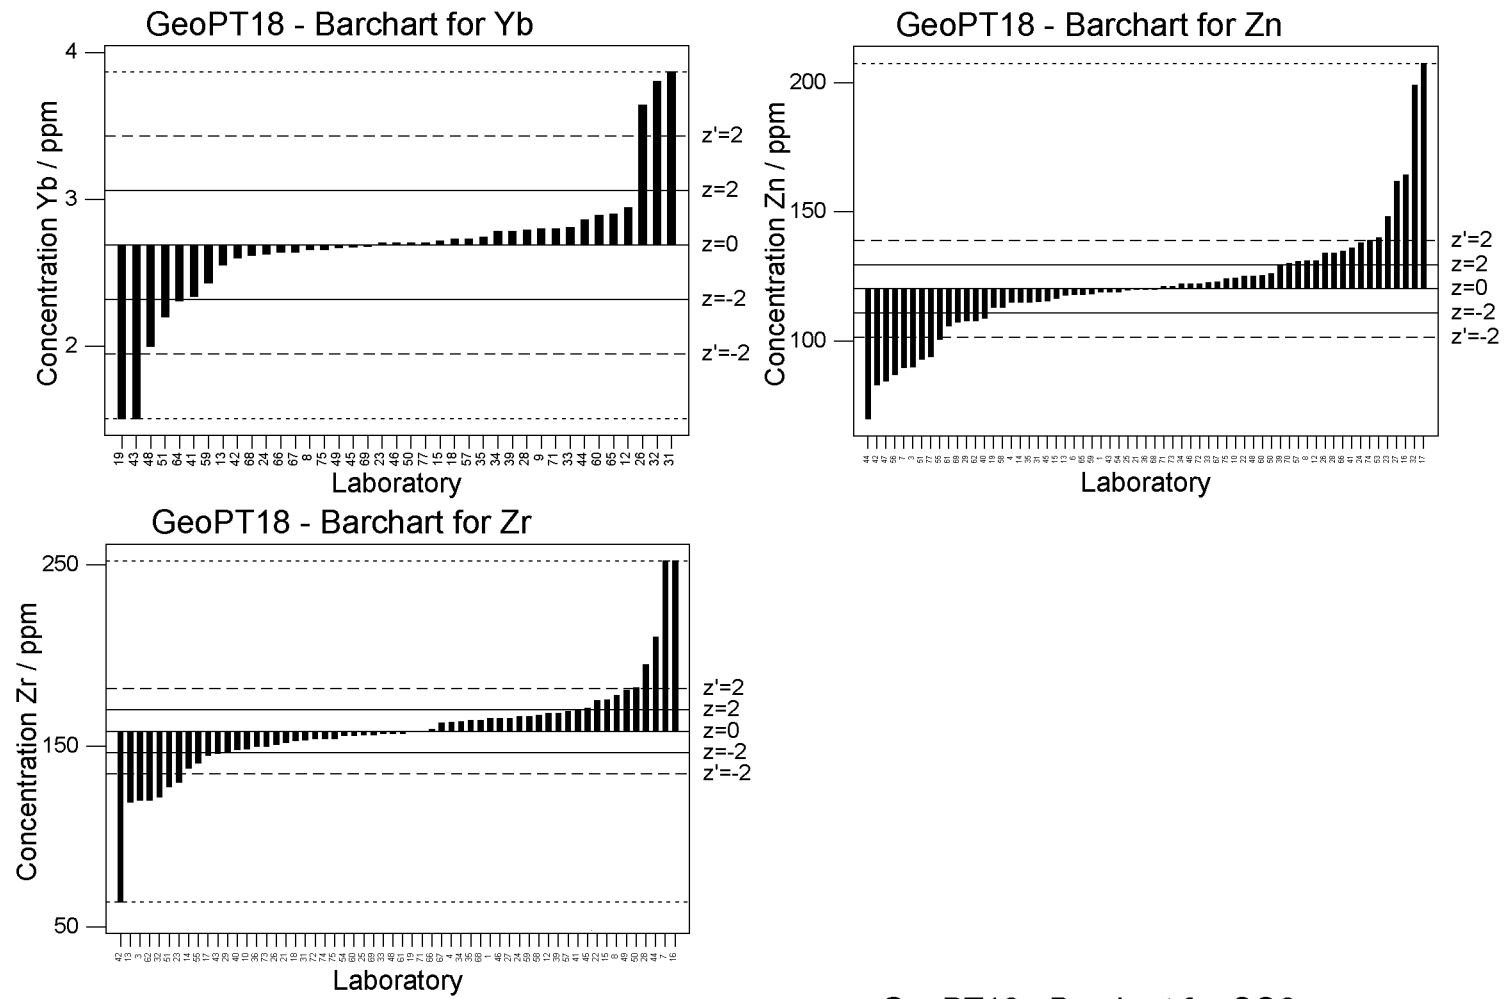


Figure 1: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

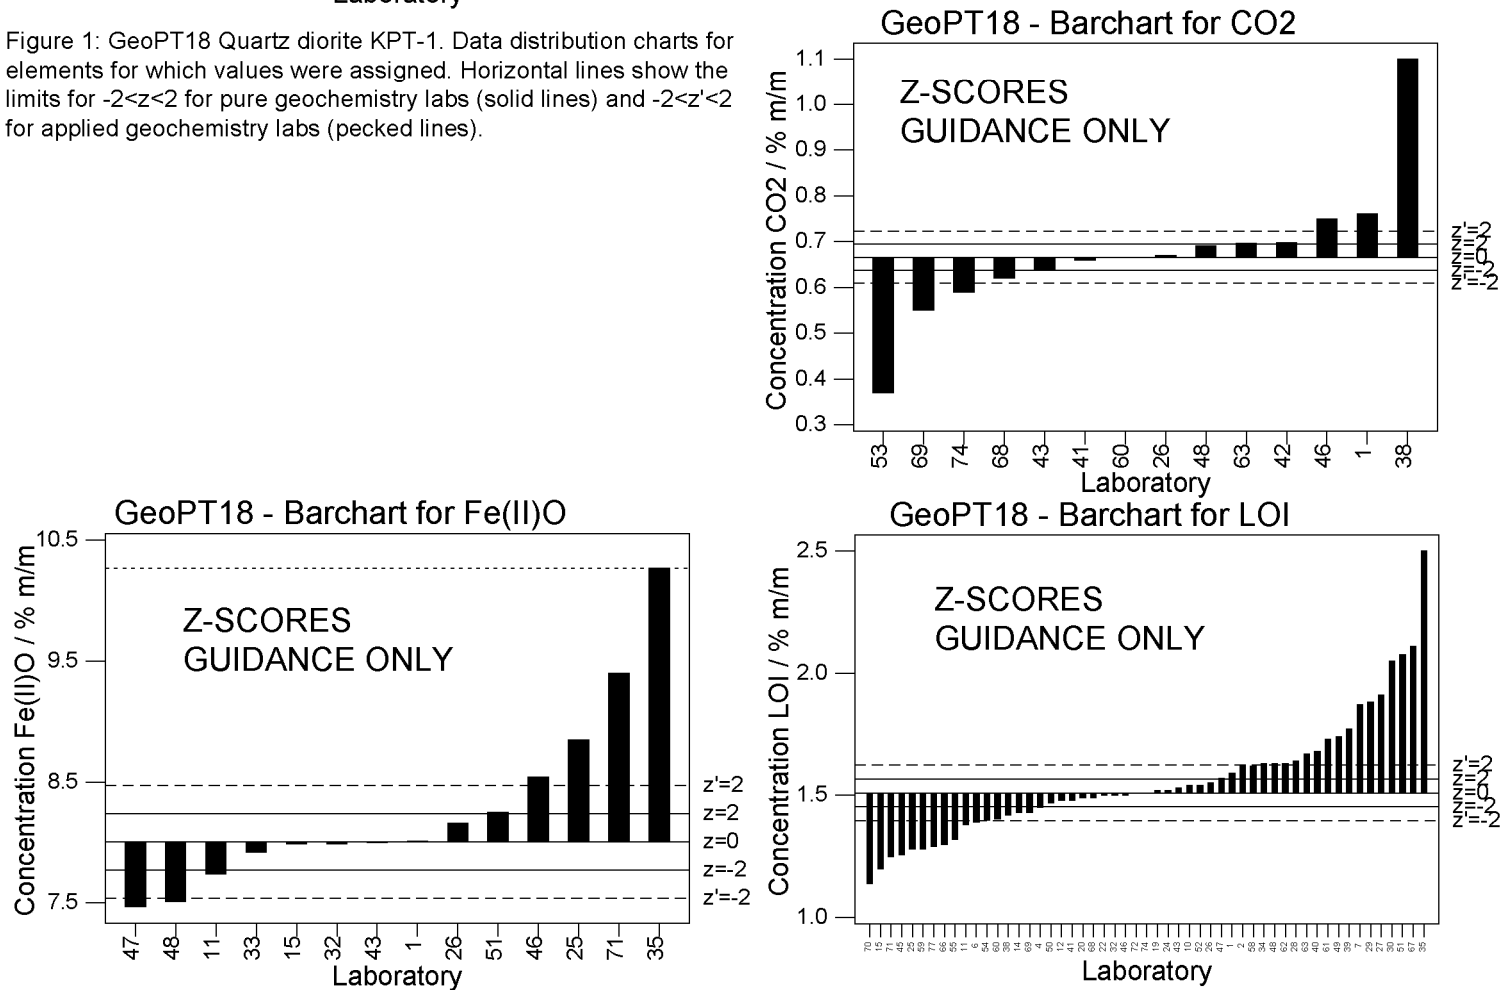


Figure 2: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which Z-scores are for guidance only. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

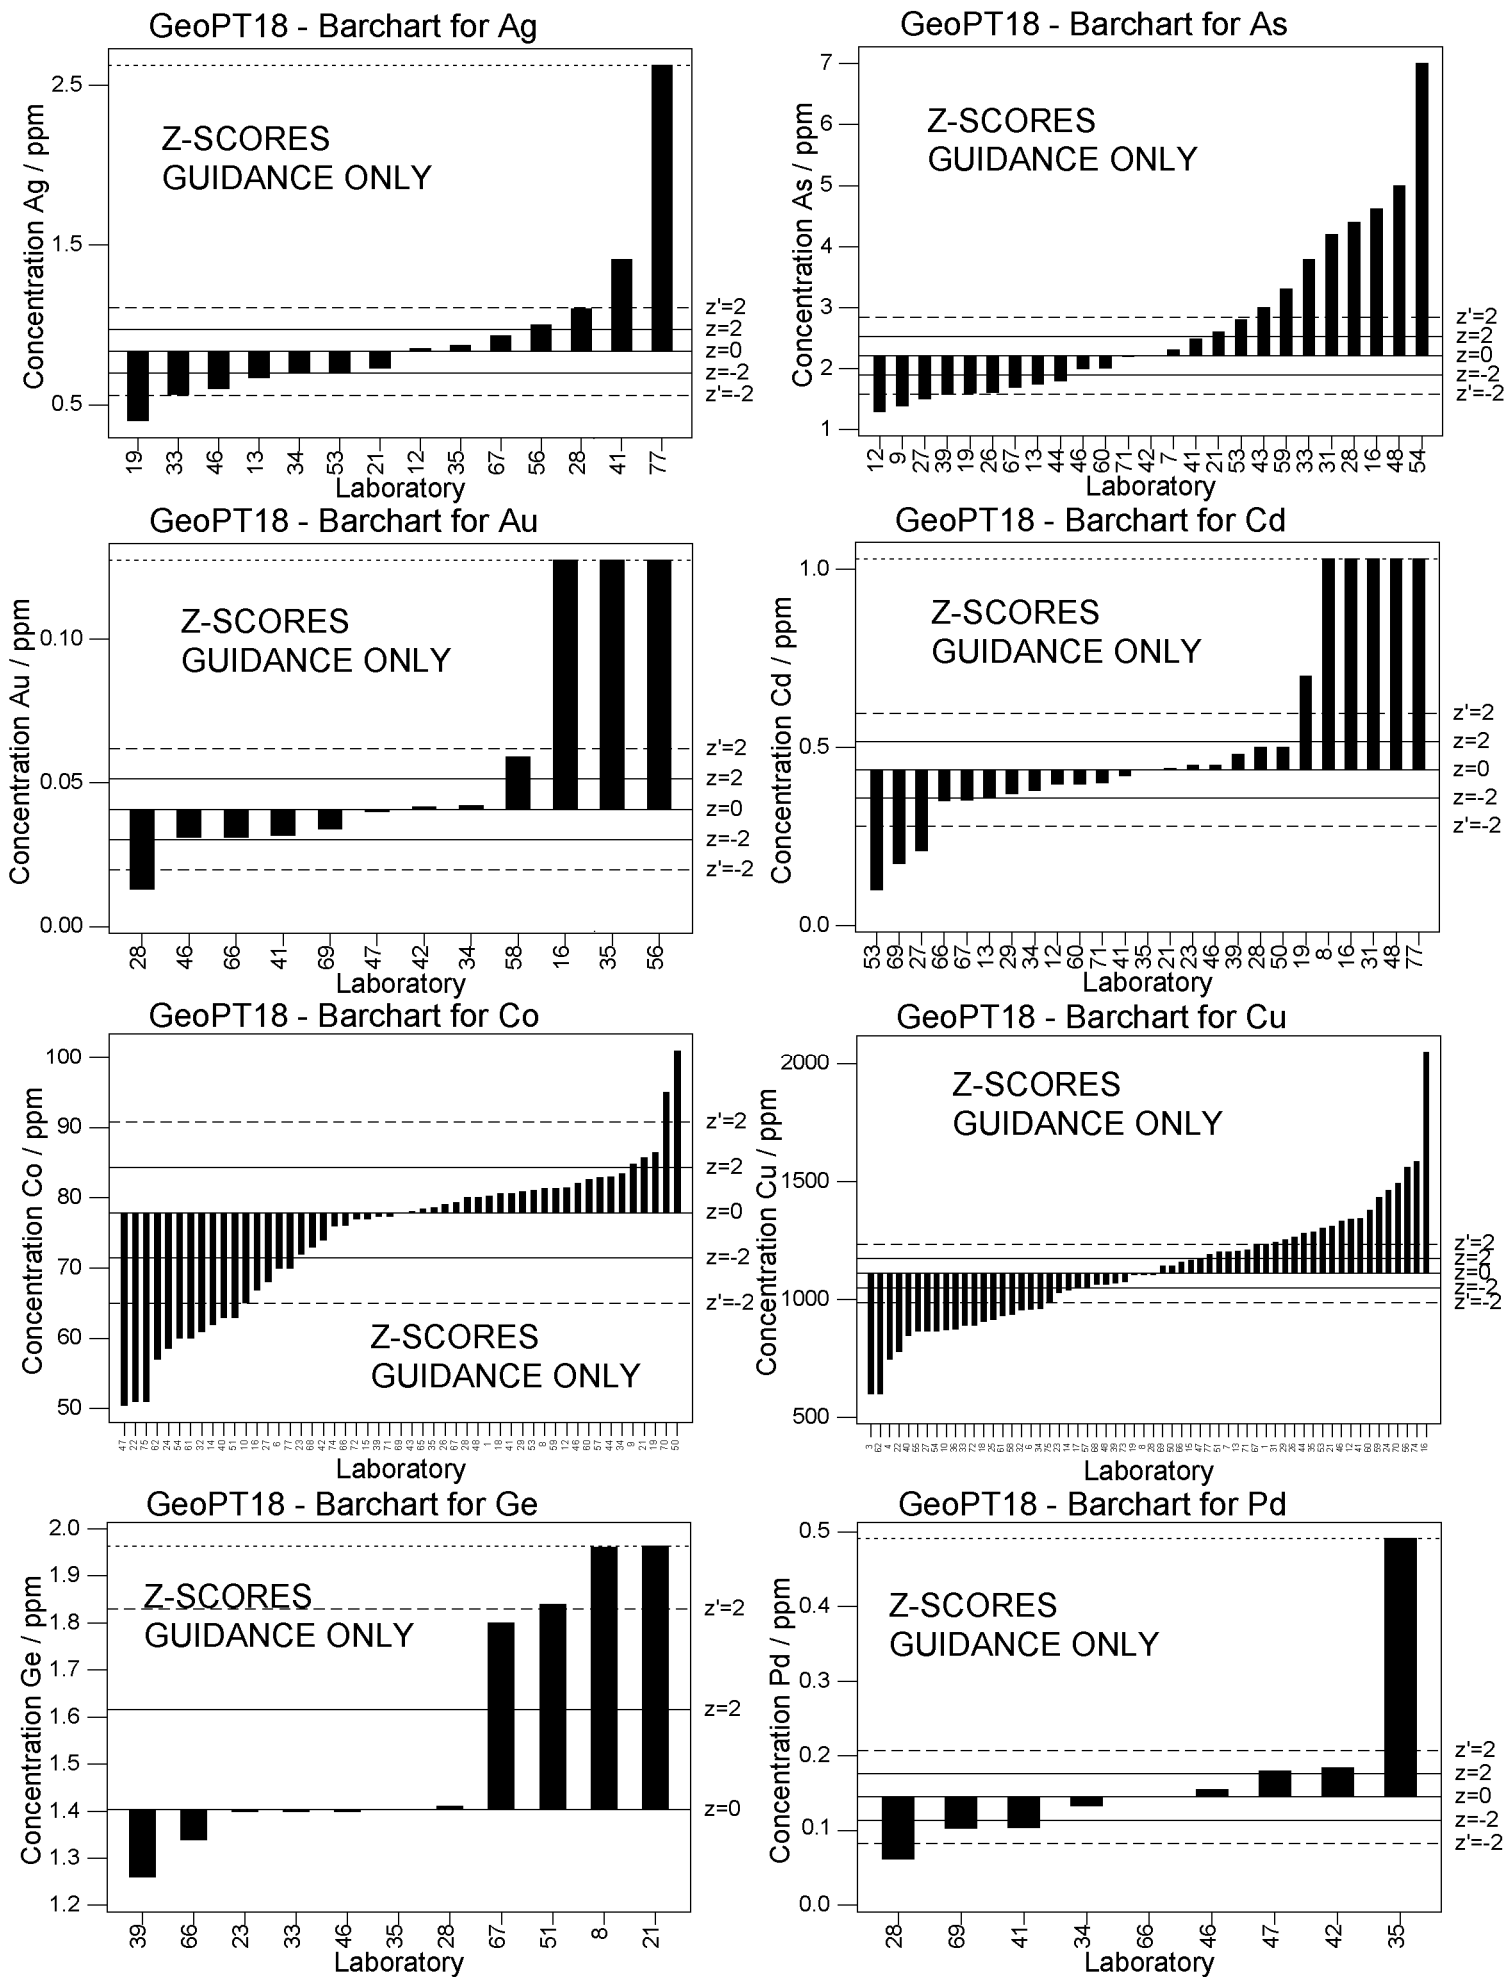


Figure 2: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values were assigned for guidance only. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

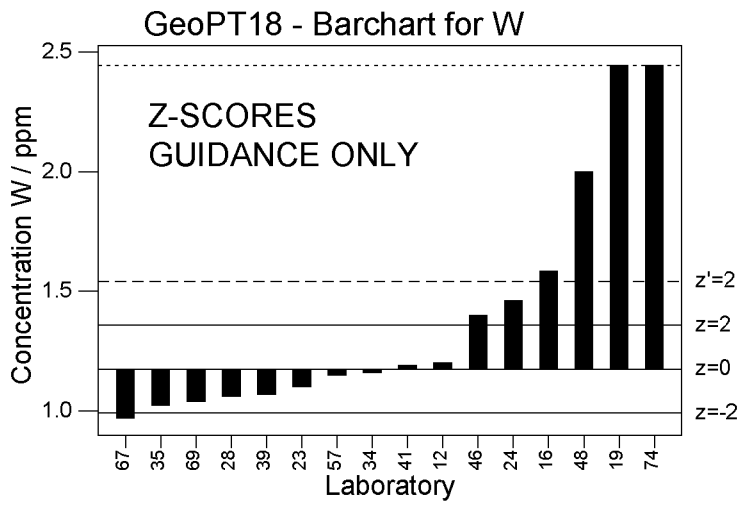


Figure 2: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which Z-scores are for guidance only. Horizontal lines show the limits for $-2 < z < 2$ for pure geochemistry labs (solid lines) and $-2 < z' < 2$ for applied geochemistry labs (pecked lines).

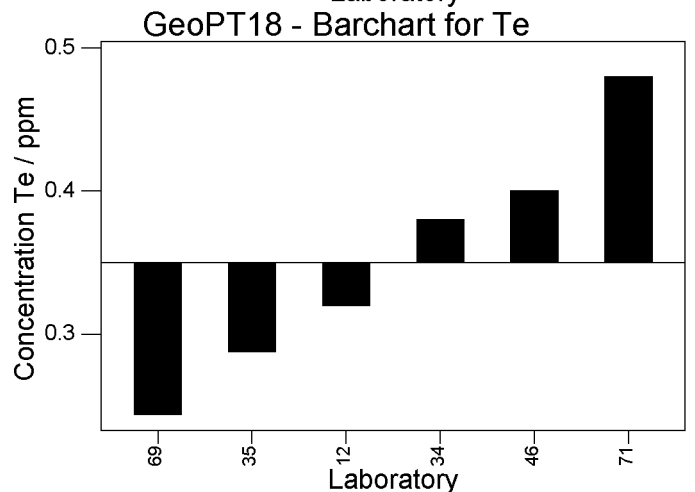
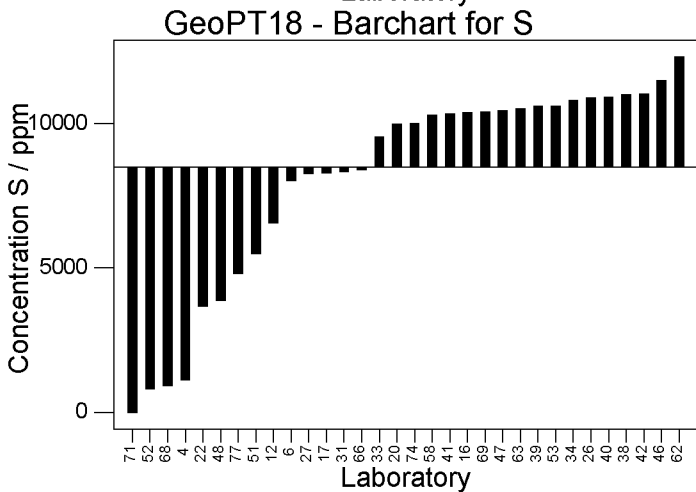
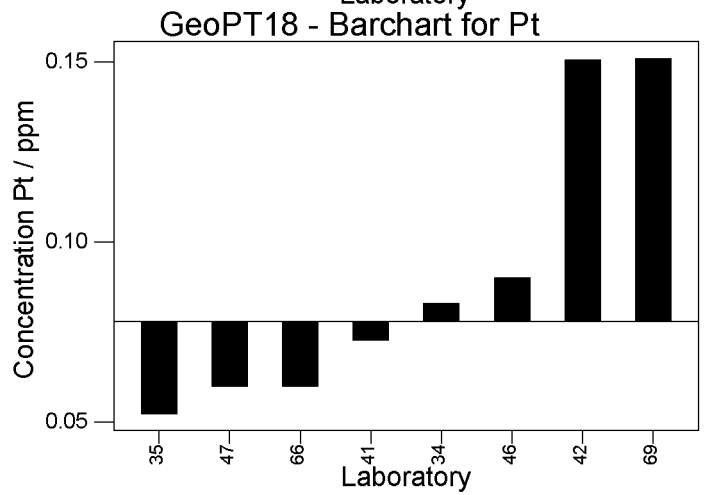
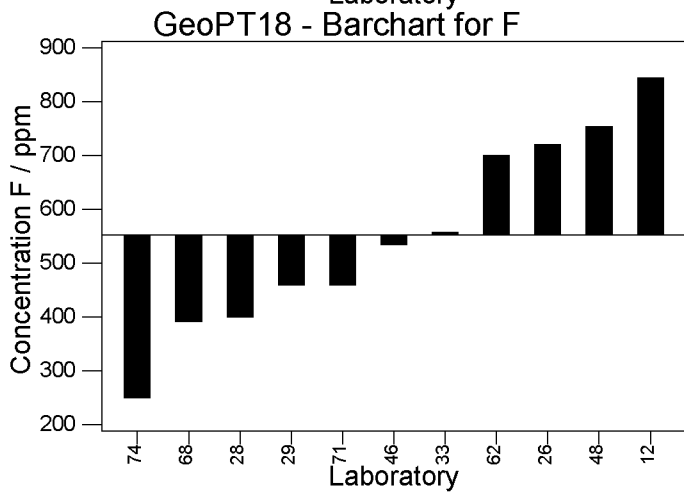
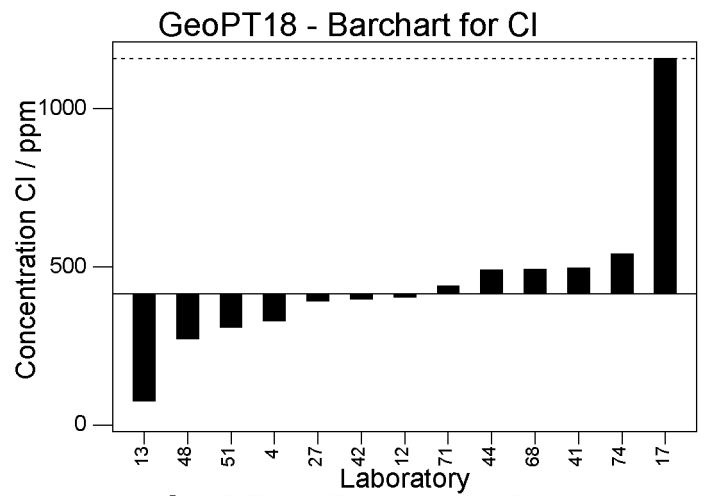
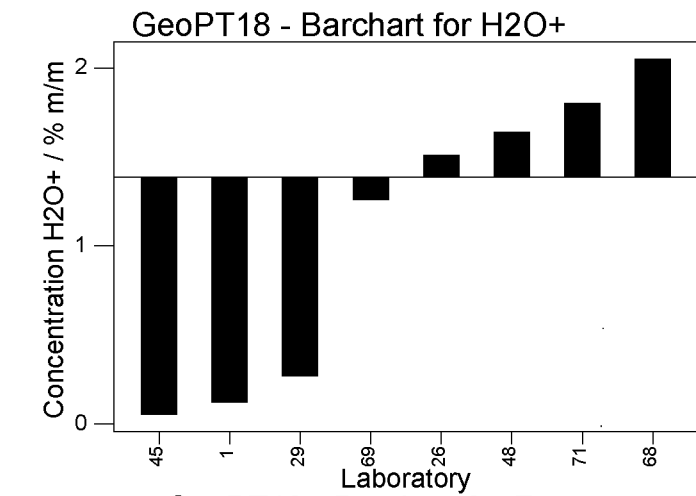


Figure 3: GeoPT18 Quartz diorite KPT-1. Data distribution charts for elements for which values could not be assigned.

Multiple z-score chart - GeoPT18

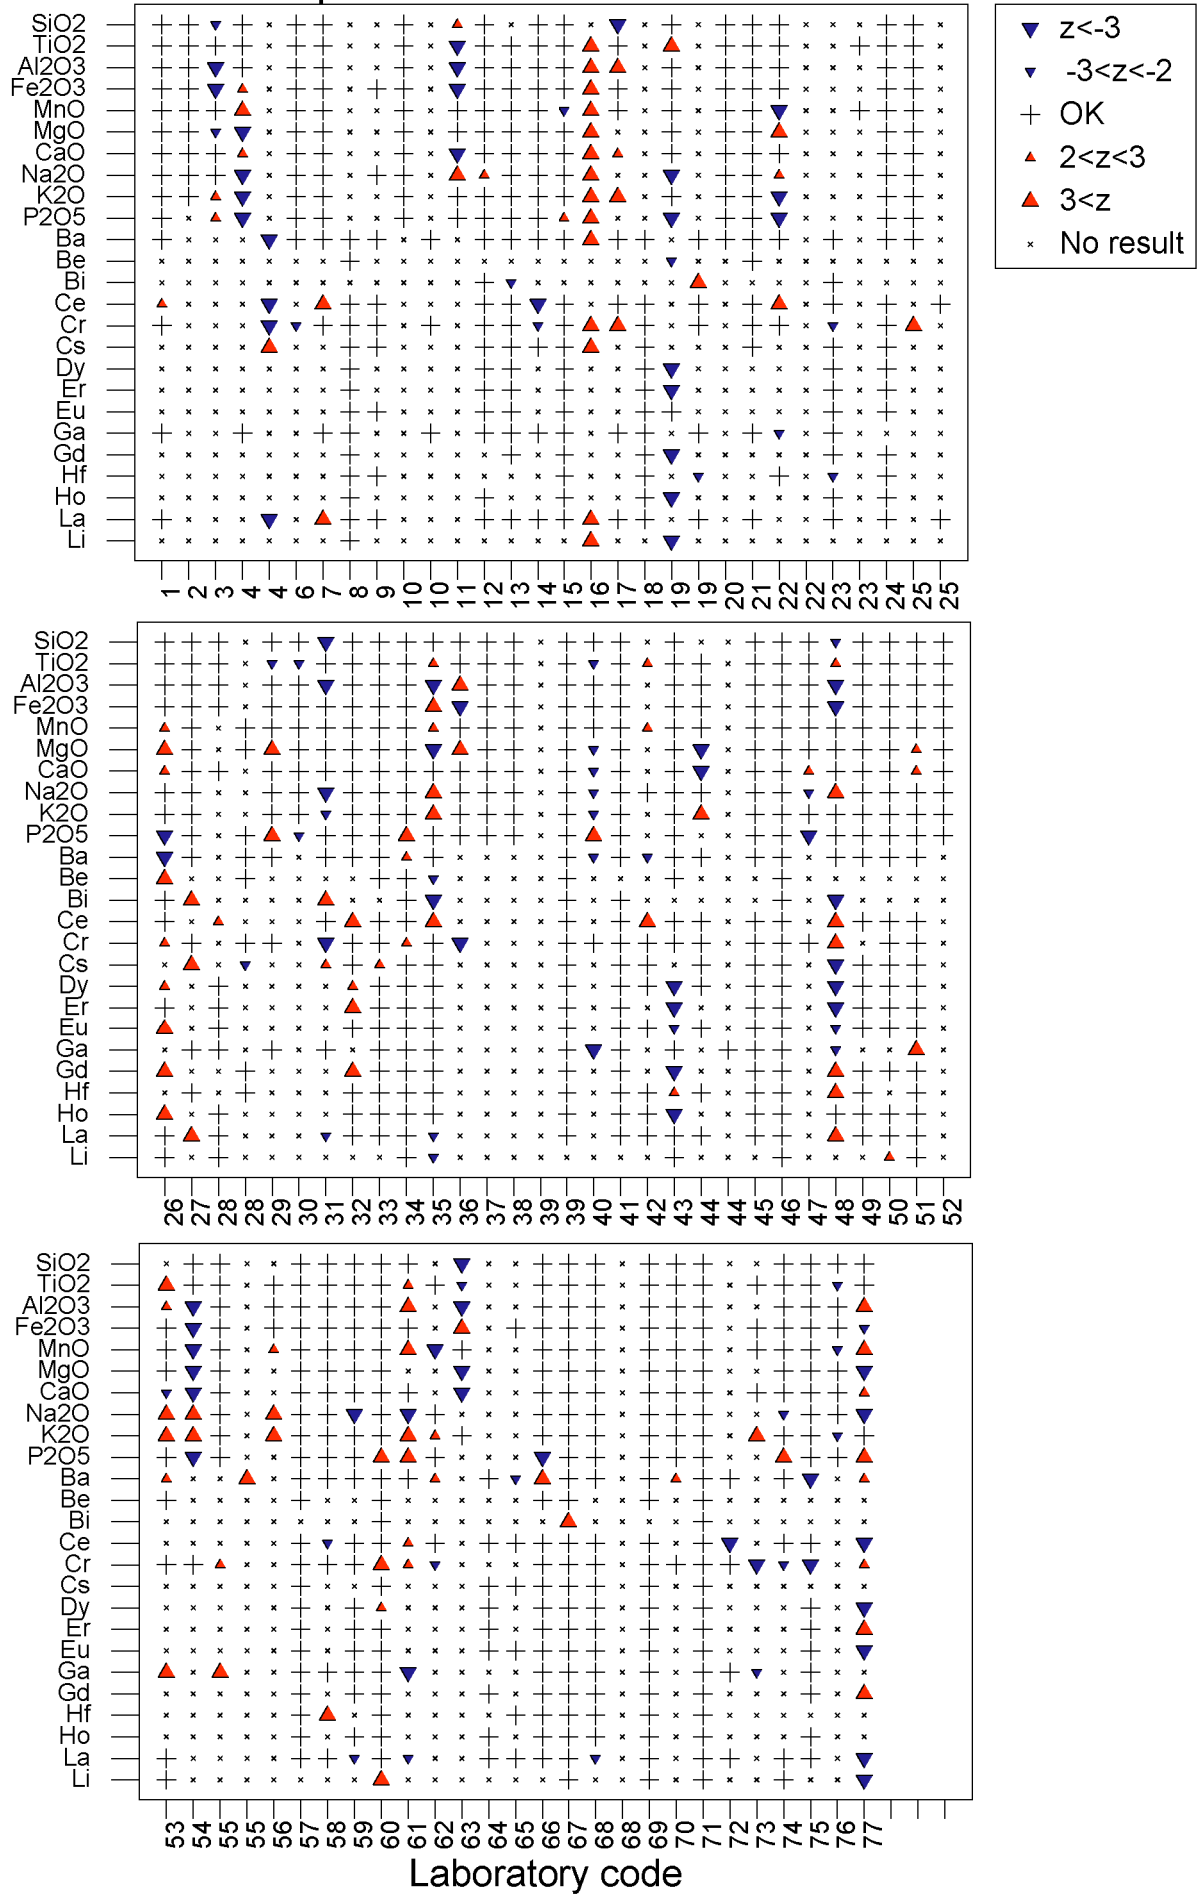


Figure 4: GeoPT18 - Quartz diorite KPT-1. Multiple z-score charts for laboratories participating in the GeoPT18 round. Symbols indicate whether or not an elemental result complies with the $-2 < z < +2$ criteria. Satisfactory data are plotted as '+'. Data for other categories are plotted as follows: $z < -3$ (t), $-3 < z < -2$ (t), $+2 < z < +3$ (s), $Z > +3$ (s).

Multiple z-score chart - GeoPT18

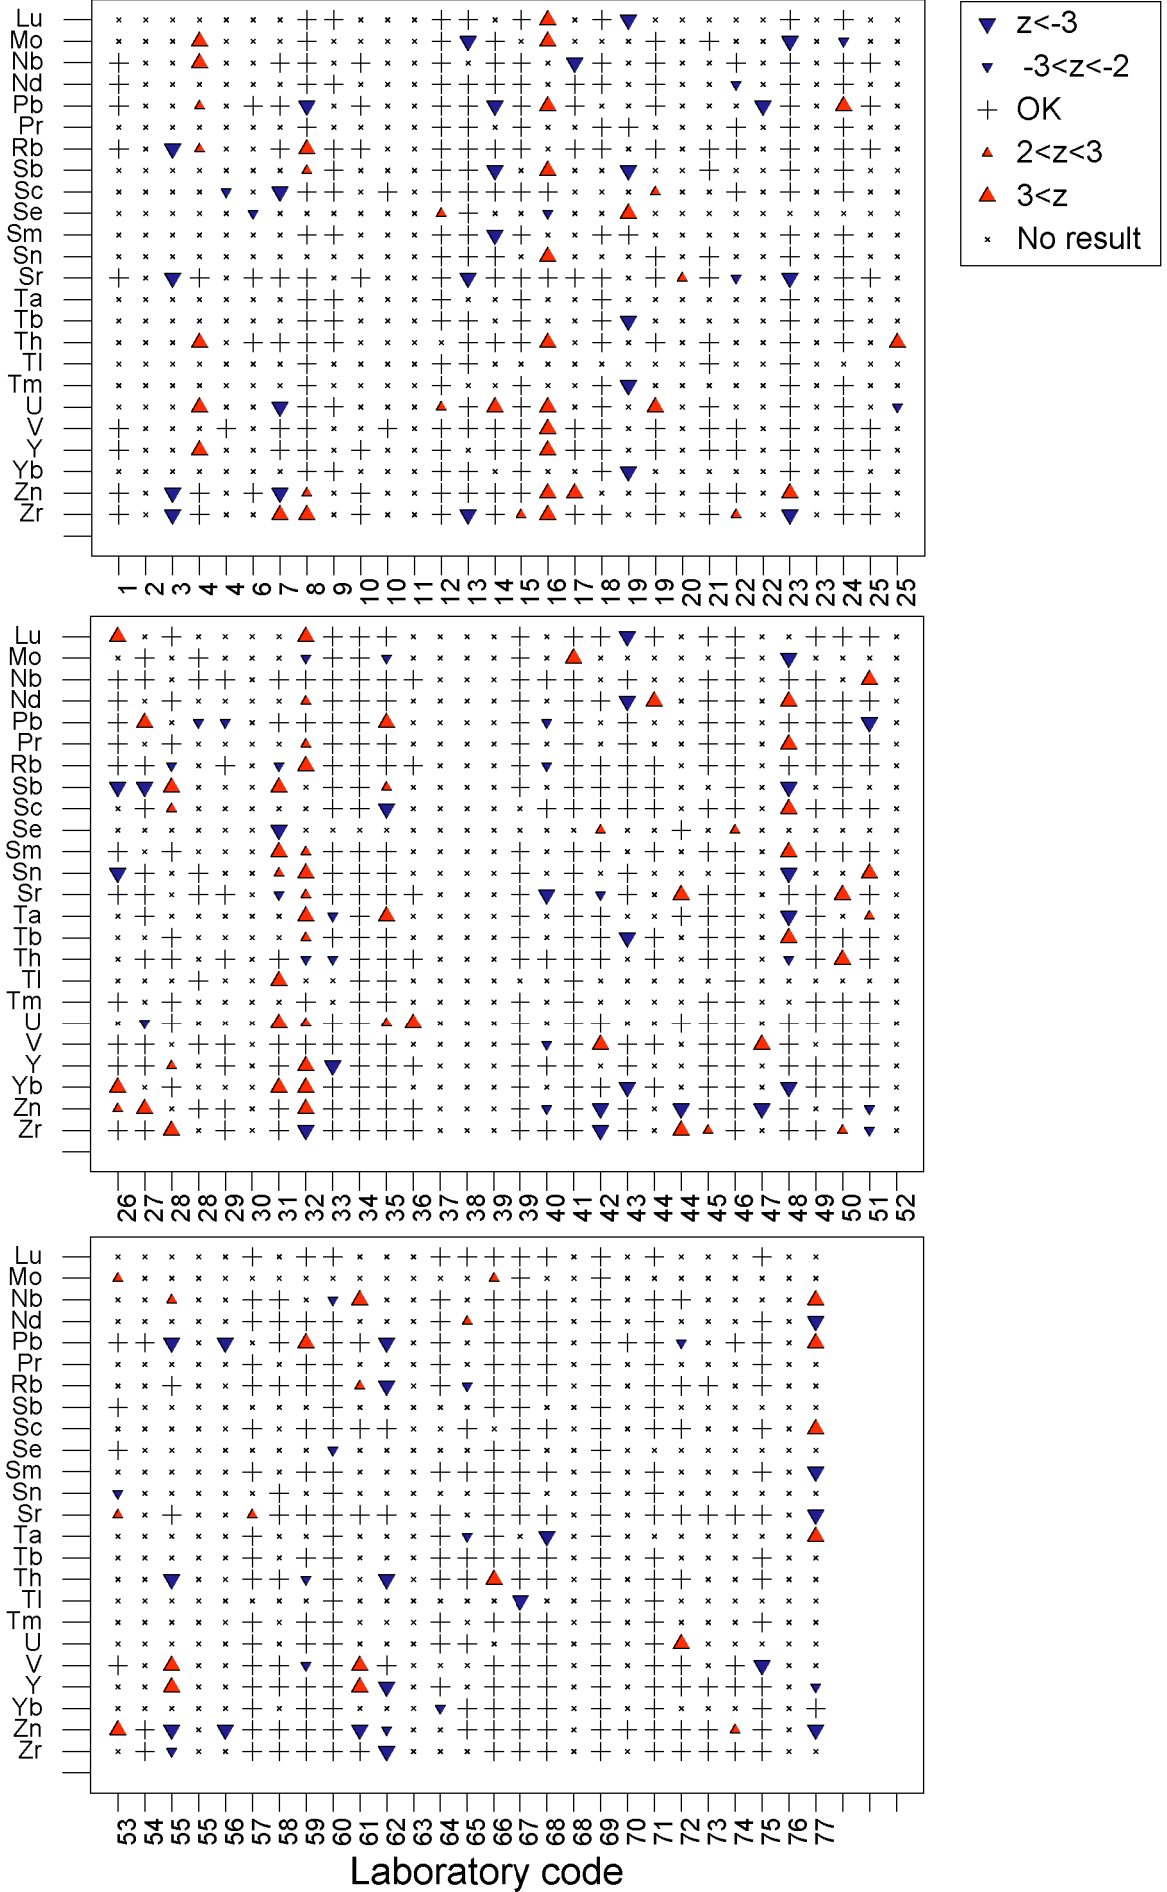


Figure 4: GeoPT18 - Quartz diorite KPT-1. Multiple z-score charts for laboratories participating in the GeoPT18 round. Symbols indicate whether or not an elemental result complies with the $-2 < z < +2$ criteria. Satisfactory data are plotted as '+'. Data for other categories are plotted as follows: $z < -3$ (t), $-3 < z < -2$ (t), $+2 < z < +3$ (s), $Z > +3$ (s).

Erratum GeoPT18

During data processing, on converting several ‘,’ separators to decimal ‘.’, for laboratory S26 the value of 1.22 ppm for Eu became 122 ppm. Consequently, the position for lab. S26 (Figure 1) in the Eu plot is represented incorrectly. The correct z-score value has been included in Table 3, however.

Note that data for two additional laboratories (S78 and S79) are recorded in Table 1 and Table 3. These data had been submitted but were not received.